

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
 Data File : VX021328.D
 Acq On : 20 Mar 2021 05:53
 Operator : JC/MD
 Sample : M1735-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE134D3-20210315

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M

Title : SW846 8260

Signal : TIC: VX021328.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.364	208	217	235	rVB	1024823	1974178	100.00%	36.996%
2	5.464	732	744	757	rBV2	52338	149279	7.56%	2.797%
3	5.629	761	772	787	rVV2	90967	251260	12.73%	4.709%
4	6.029	829	840	851	rBV2	63109	163351	8.27%	3.061%
5	6.829	965	976	987	rBV	136970	323770	16.40%	6.067%
6	7.188	1026	1037	1055	rBV	378725	801464	40.60%	15.019%
7	8.694	1284	1293	1303	rBV	274885	433888	21.98%	8.131%
8	9.318	1392	1399	1412	rVB	217854	318280	16.12%	5.965%
9	10.094	1525	1531	1548	rVB	264675	358935	18.18%	6.726%
10	11.118	1700	1705	1716	rVB	207457	266695	13.51%	4.998%
11	12.059	1860	1865	1871	rBV	240676	295113	14.95%	5.530%




Sum of corrected areas: 5336213

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
Data File : VX021328.D
Acq On : 20 Mar 2021 05:53
Operator : JC/MD
Sample : M1735-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE134D3-20210315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

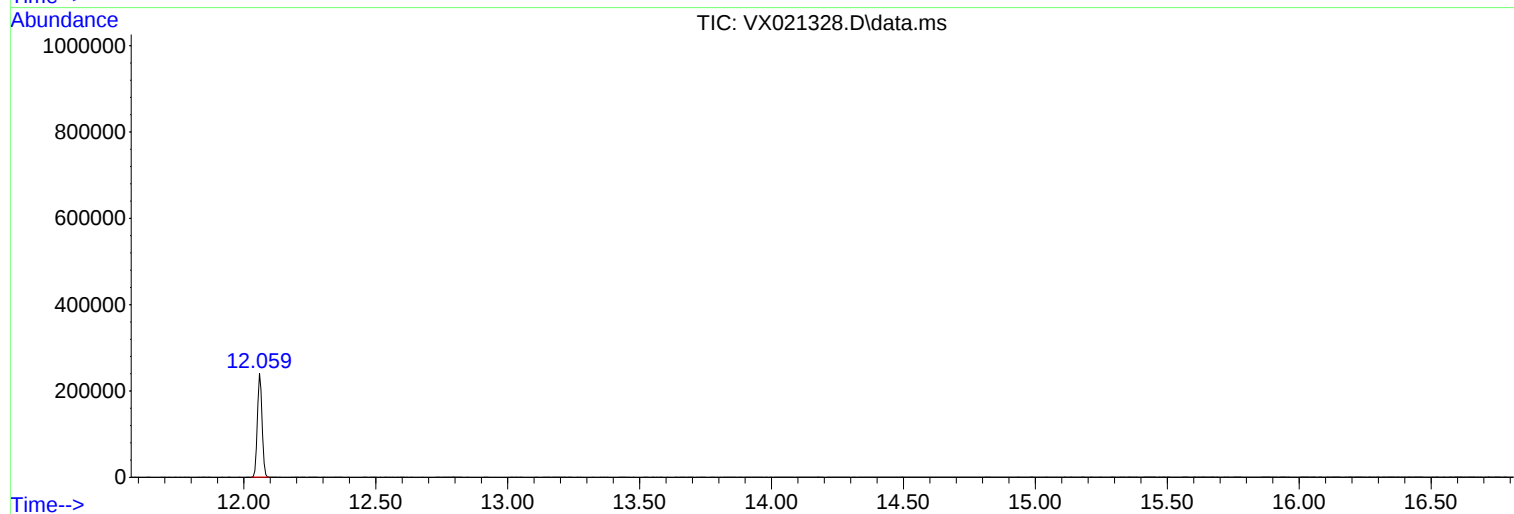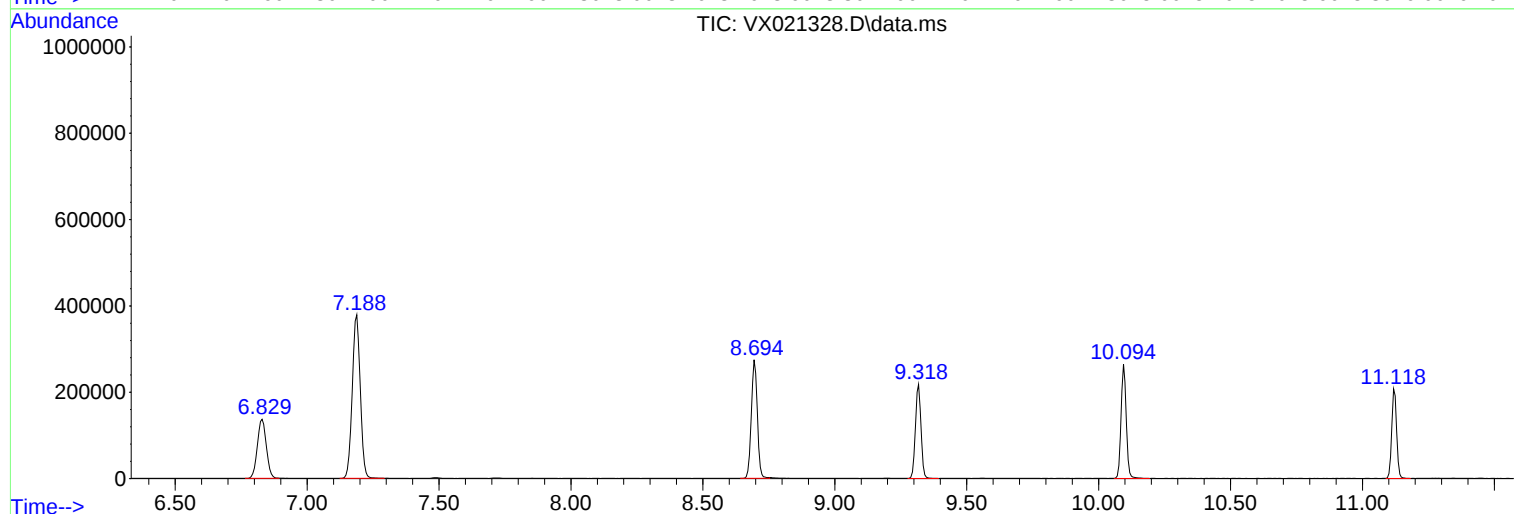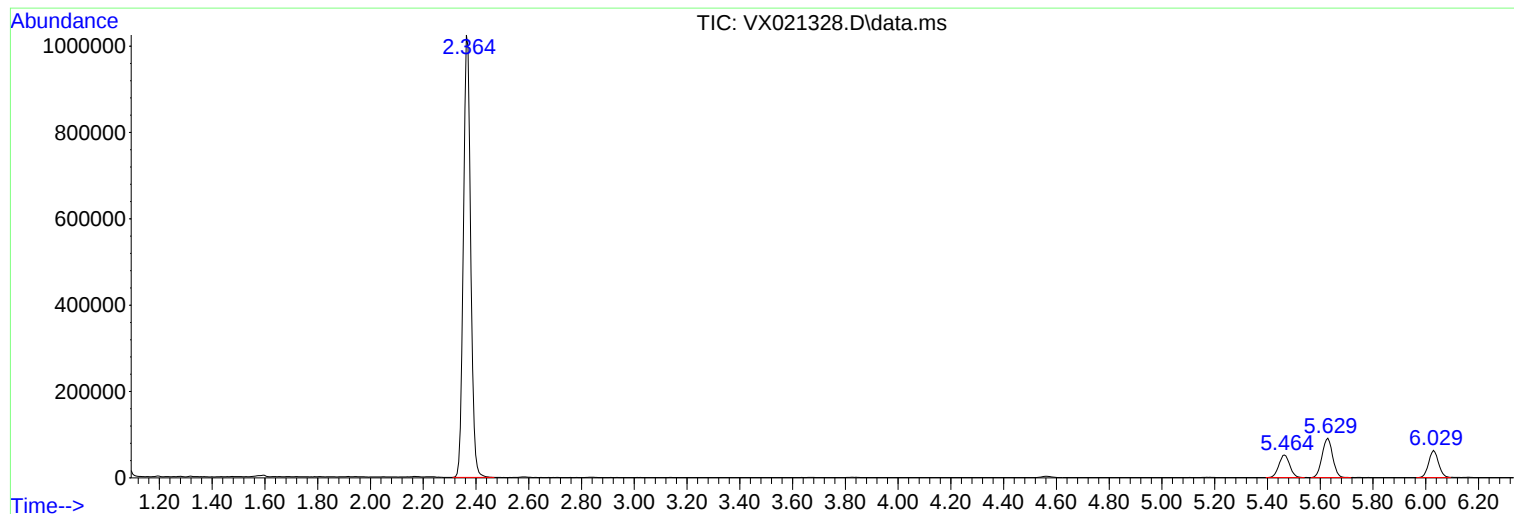

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
Data File : VX021328.D
Acq On : 20 Mar 2021 05:53
Operator : JC/MD
Sample : M1735-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE134D3-20210315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
Data File : VX021328.D
Acq On : 20 Mar 2021 05:53
Operator : JC/MD
Sample : M1735-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE134D3-20210315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
