

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
 Data File : VX021330.D
 Acq On : 20 Mar 2021 06:39
 Operator : JC/MD
 Sample : M1735-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE132D5-20210315

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M

Title : SW846 8260

Signal : TIC: VX021330.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.364	210	217	225	rBV3	28834	54544	8.26%	1.785%
2	4.564	580	591	602	rBV3	3411	8609	1.30%	0.282%
3	5.464	733	744	759	rBV	54706	156623	23.72%	5.125%
4	5.629	761	772	786	rVV2	92503	256570	38.85%	8.395%
5	6.029	827	840	854	rBV	63767	170052	25.75%	5.564%
6	6.829	965	976	991	rBV	141245	334510	50.65%	10.946%
7	7.188	1026	1037	1048	rBV	316062	660376	100.00%	21.608%
8	8.694	1286	1293	1302	rBV	291882	453132	68.62%	14.827%
9	10.094	1525	1531	1541	rBV	273656	372437	56.40%	12.187%
10	11.118	1700	1705	1715	rVB	218286	280277	42.44%	9.171%
11	12.059	1859	1865	1874	rVB	255642	308986	46.79%	10.110%




Sum of corrected areas: 3056116

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
Data File : VX021330.D
Acq On : 20 Mar 2021 06:39
Operator : JC/MD
Sample : M1735-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D5-20210315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

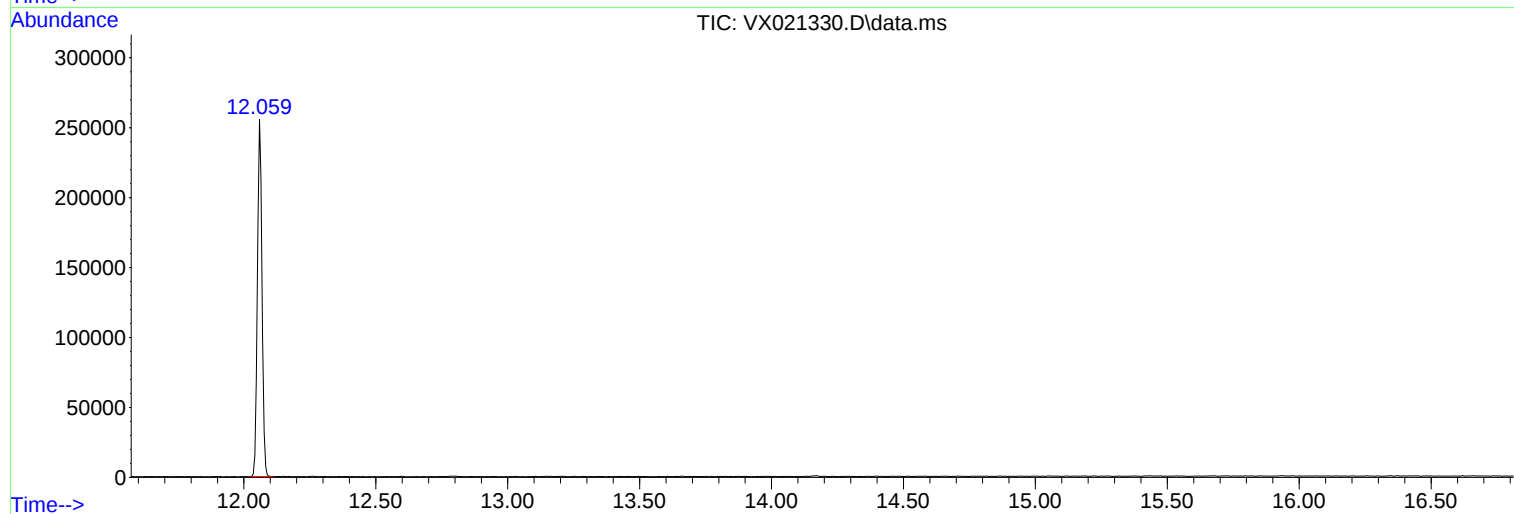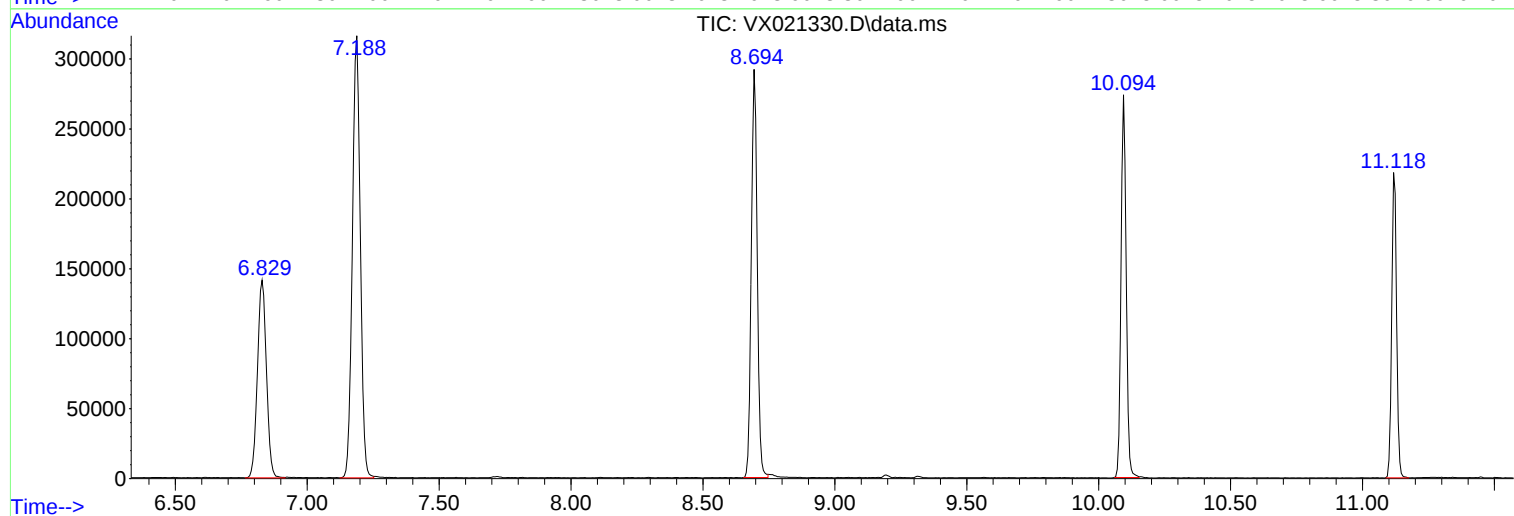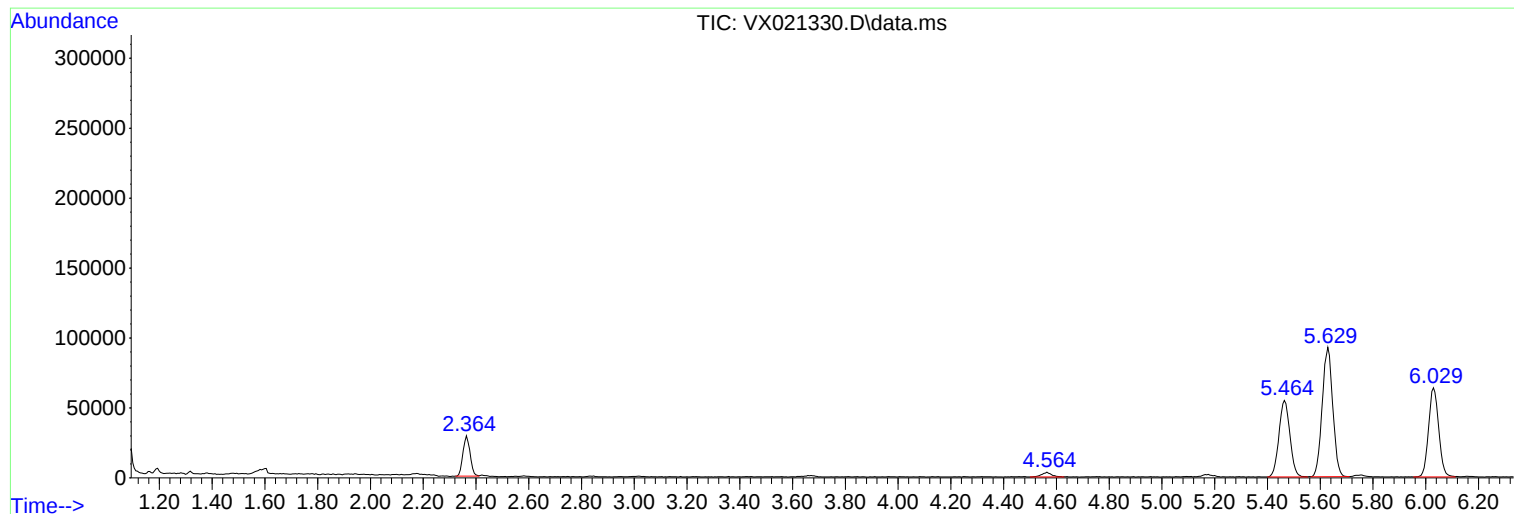

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
Data File : VX021330.D
Acq On : 20 Mar 2021 06:39
Operator : JC/MD
Sample : M1735-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D5-20210315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
Data File : VX021330.D
Acq On : 20 Mar 2021 06:39
Operator : JC/MD
Sample : M1735-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D5-20210315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
