

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
 Data File : VX021338.D
 Acq On : 20 Mar 2021 09:46
 Operator : JC/MD
 Sample : M1735-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE131D3-20210317

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
 Title : SW846 8260

Signal : TIC: VX021338.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.364	209	217	235	rVB	726163	1408394	100.00%	35.548%
2	5.464	732	744	757	rBV	54716	156144	11.09%	3.941%
3	5.629	760	772	786	rVV	92420	257530	18.29%	6.500%
4	6.029	828	840	852	rBV	63580	168362	11.95%	4.250%
5	6.829	962	976	988	rBV	141623	334376	23.74%	8.440%
6	7.188	1024	1037	1046	rBV	70385	149069	10.58%	3.763%
7	8.694	1285	1293	1313	rBV	285439	455203	32.32%	11.490%
8	9.317	1393	1399	1409	rVB	50102	73176	5.20%	1.847%
9	10.094	1525	1531	1548	rVB	269651	376177	26.71%	9.495%
10	11.118	1700	1705	1716	rVB	211114	277897	19.73%	7.014%
11	12.059	1860	1865	1872	rBV	246799	305574	21.70%	7.713%




Sum of corrected areas: 3961902

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
Data File : VX021338.D
Acq On : 20 Mar 2021 09:46
Operator : JC/MD
Sample : M1735-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE131D3-20210317

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

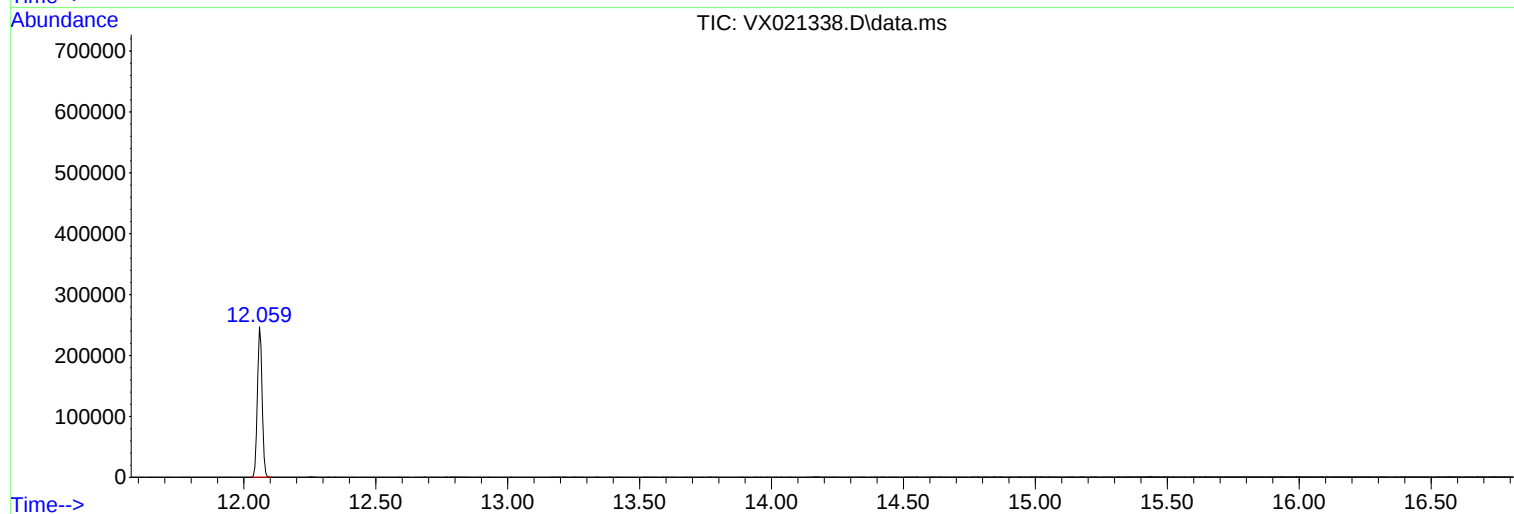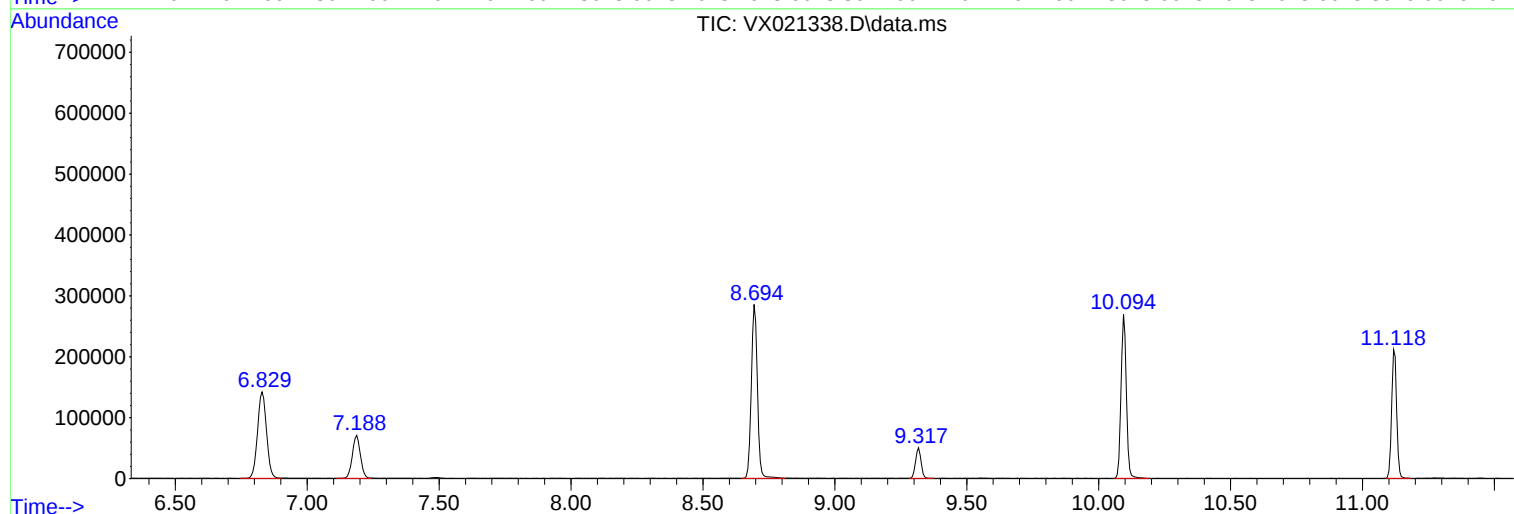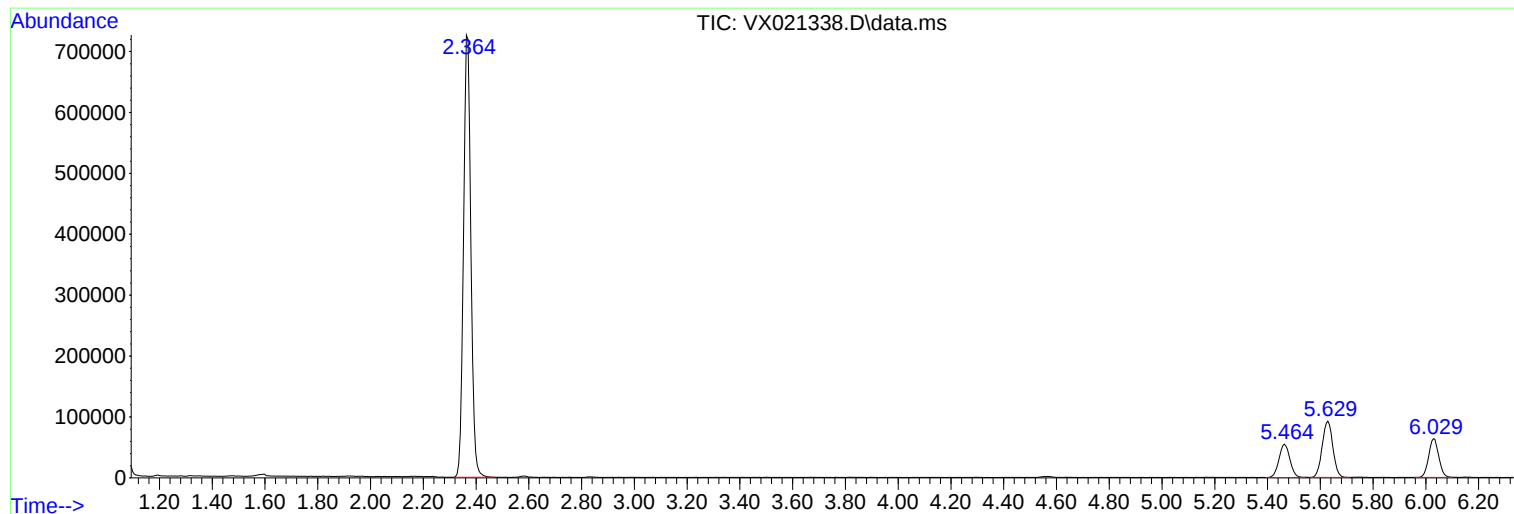

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
Data File : VX021338.D
Acq On : 20 Mar 2021 09:46
Operator : JC/MD
Sample : M1735-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE131D3-20210317

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
Data File : VX021338.D
Acq On : 20 Mar 2021 09:46
Operator : JC/MD
Sample : M1735-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE131D3-20210317

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
