

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
 Data File : VX021340.D
 Acq On : 20 Mar 2021 10:33
 Operator : JC/MD
 Sample : M1735-22
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE135D1-20210317

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
 Title : SW846 8260

Signal : TIC: VX021340.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	77	87	90	rBV5	3545	7475	1.76%	0.337%
2	2.576	248	253	264	rVB2	2284	4619	1.09%	0.208%
3	5.176	685	695	704	rVB2	2724	7663	1.80%	0.346%
4	5.464	730	744	759	rBV2	50353	144257	33.93%	6.508%
5	5.623	761	771	788	rVV	87229	242575	57.05%	10.944%
6	6.029	829	840	856	rBV	60176	157168	36.97%	7.091%
7	6.829	966	976	988	rBV	134094	309074	72.69%	13.944%
8	8.694	1286	1293	1309	rBV	276212	425170	100.00%	19.182%
9	10.094	1525	1531	1547	rVB	258877	355517	83.62%	16.039%
10	11.118	1699	1705	1714	rBV	207594	265941	62.55%	11.998%
11	12.059	1860	1865	1875	rVB	241399	297058	69.87%	13.402%




Sum of corrected areas: 2216517

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
Data File : VX021340.D
Acq On : 20 Mar 2021 10:33
Operator : JC/MD
Sample : M1735-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE135D1-20210317

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

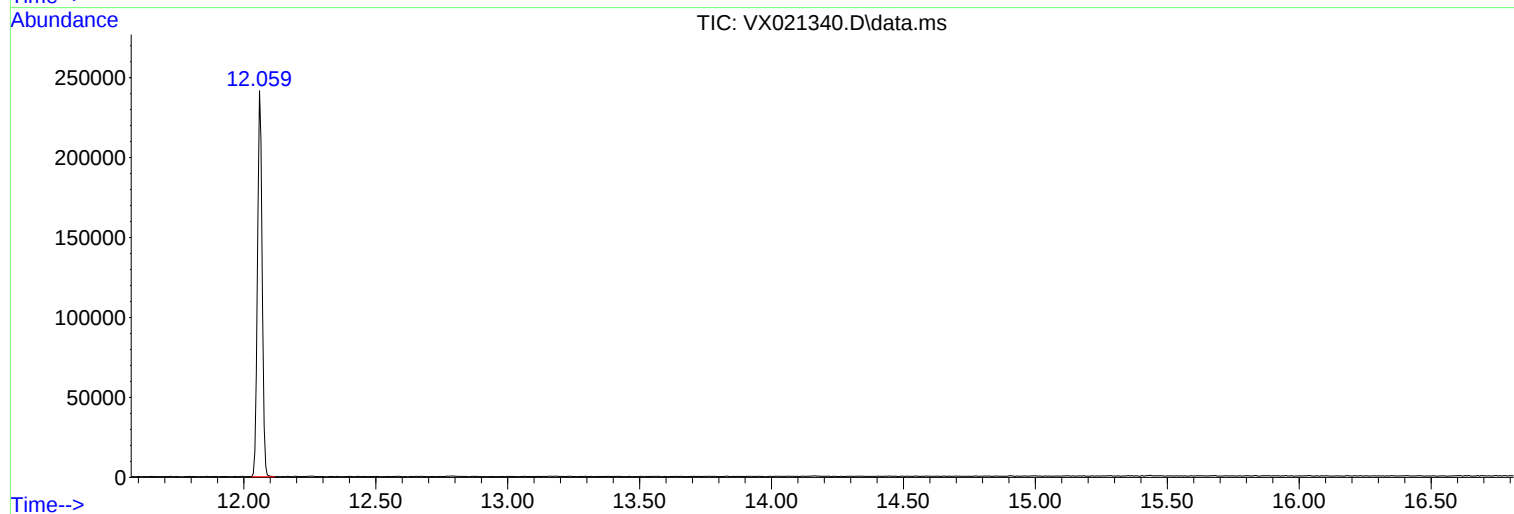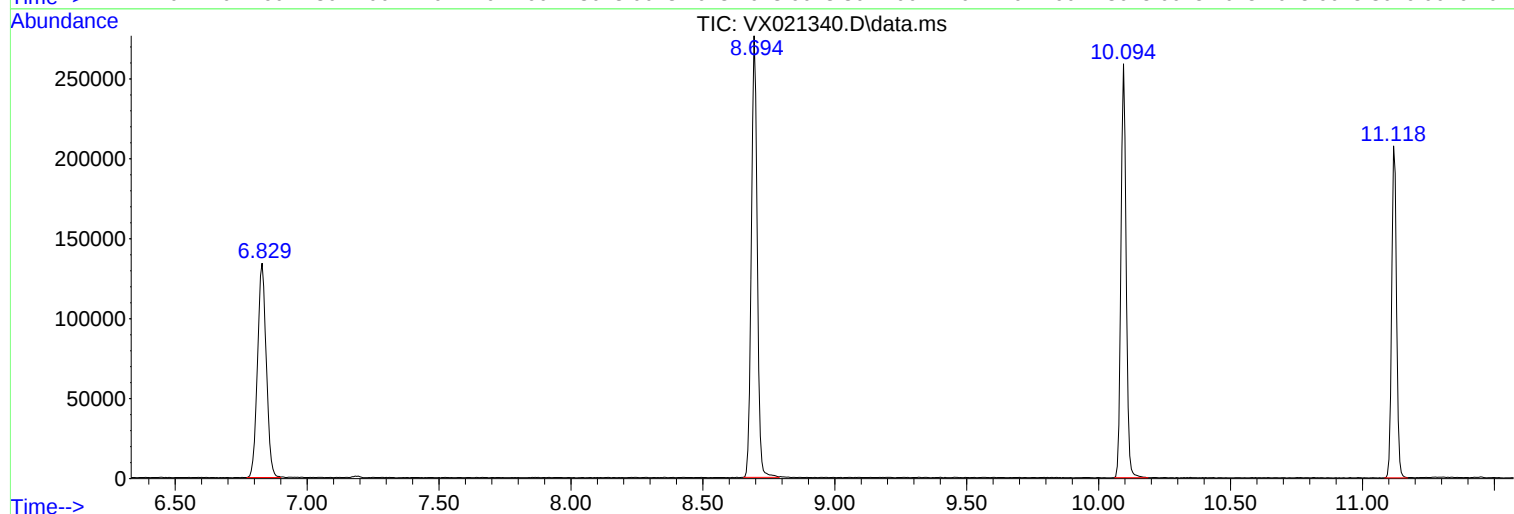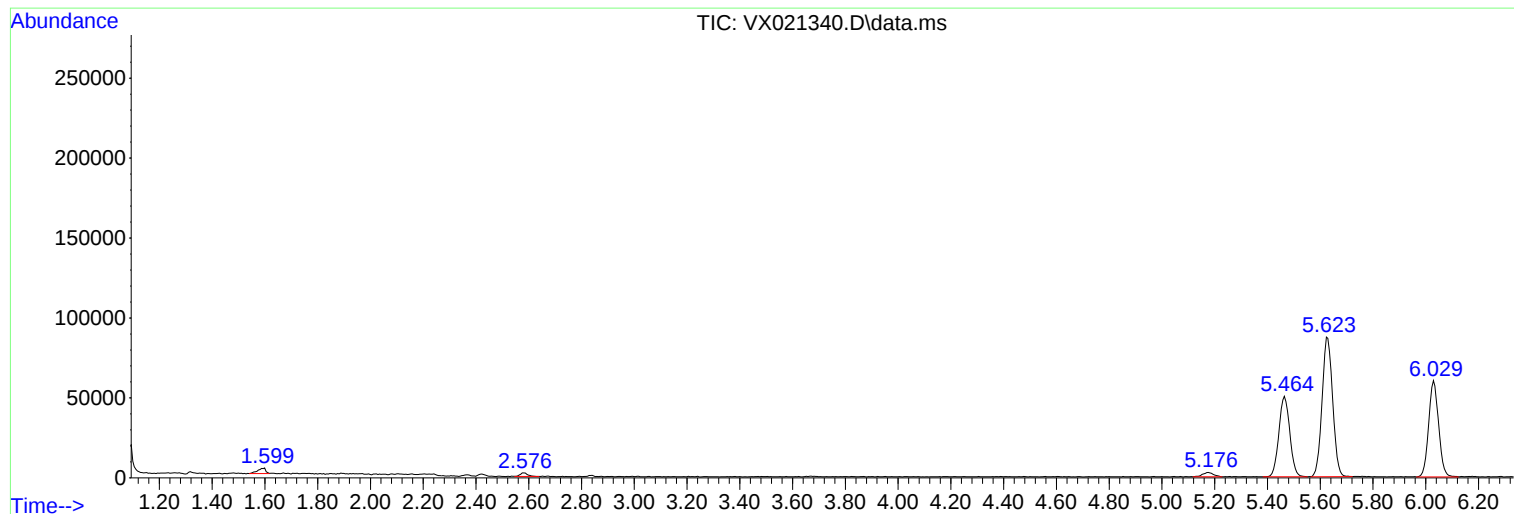

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
Data File : VX021340.D
Acq On : 20 Mar 2021 10:33
Operator : JC/MD
Sample : M1735-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE135D1-20210317

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
Data File : VX021340.D
Acq On : 20 Mar 2021 10:33
Operator : JC/MD
Sample : M1735-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE135D1-20210317

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
