


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
 Data File : VX021297.D
 Acq On : 19 Mar 2021 12:23
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
 Title : SW846 8260
 Last Update : Tue Mar 16 14:00:21 2021

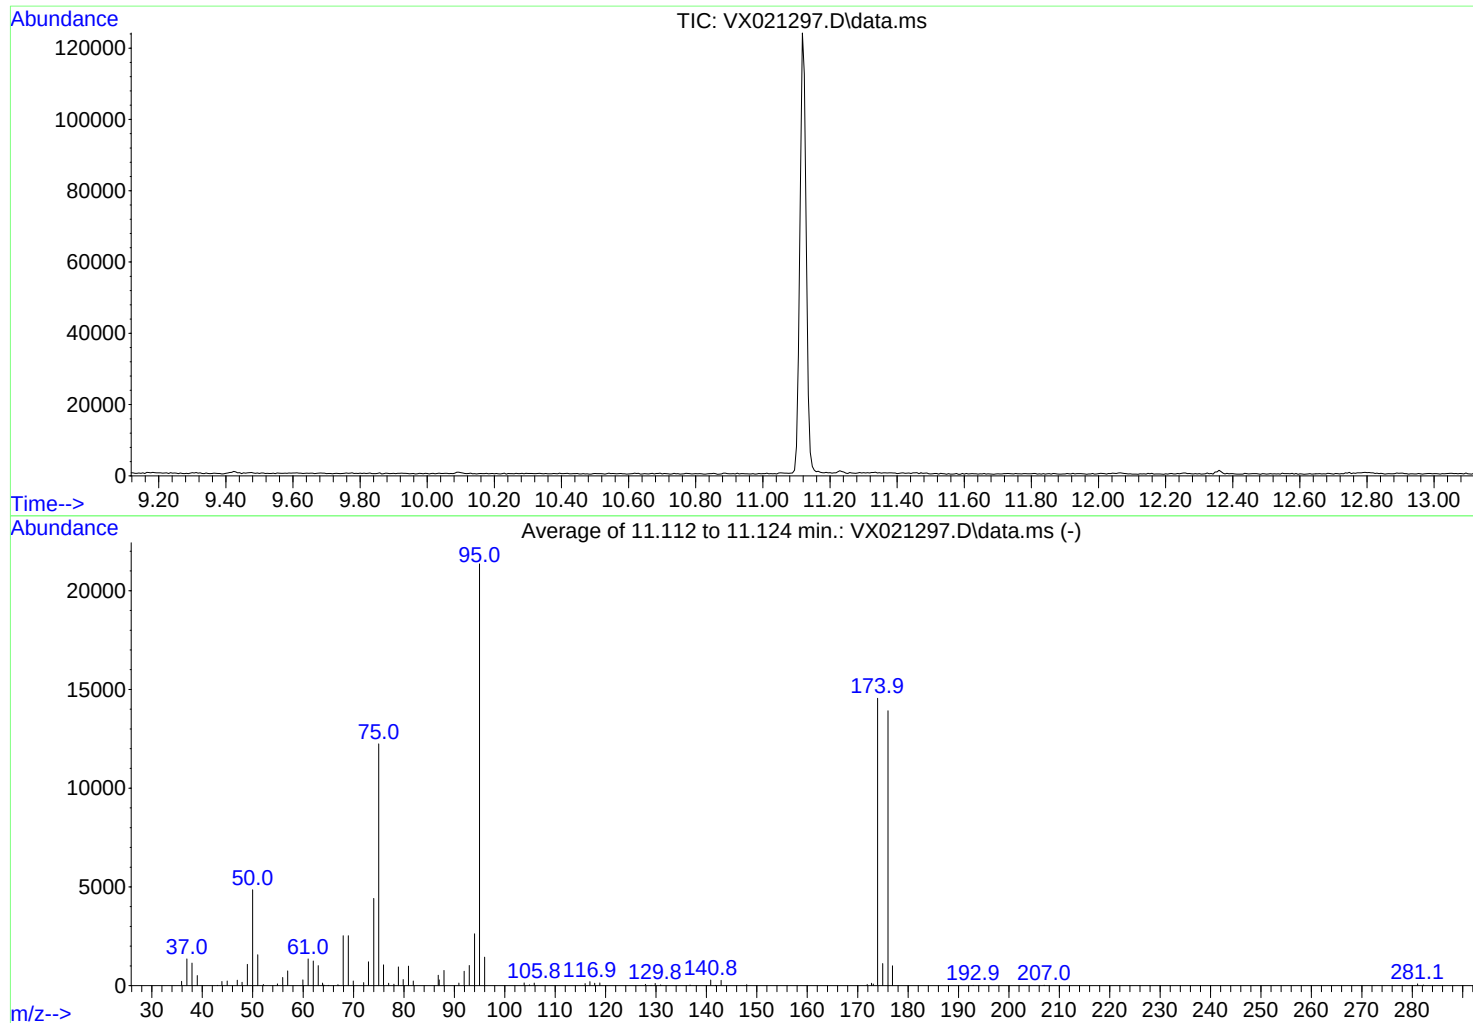

AutoFind: Scans 1704, 1705, 1706; Background Corrected with Scan 1697

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	4855	PASS
75	95	30	60	57.3	12240	PASS
95	95	100	100	100.0	21360	PASS
96	95	5	9	6.7	1439	PASS
173	174	0.00	2	0.8	120	PASS
174	95	50	100	68.1	14554	PASS
175	174	5	9	7.7	1122	PASS
176	174	95	101	95.6	13919	PASS
177	176	5	9	7.2	1003	PASS