


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032121\
 Data File : VX021320.D
 Acq On : 20 Mar 2021 01:19
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
 Title : SW846 8260
 Last Update : Tue Mar 16 14:00:21 2021

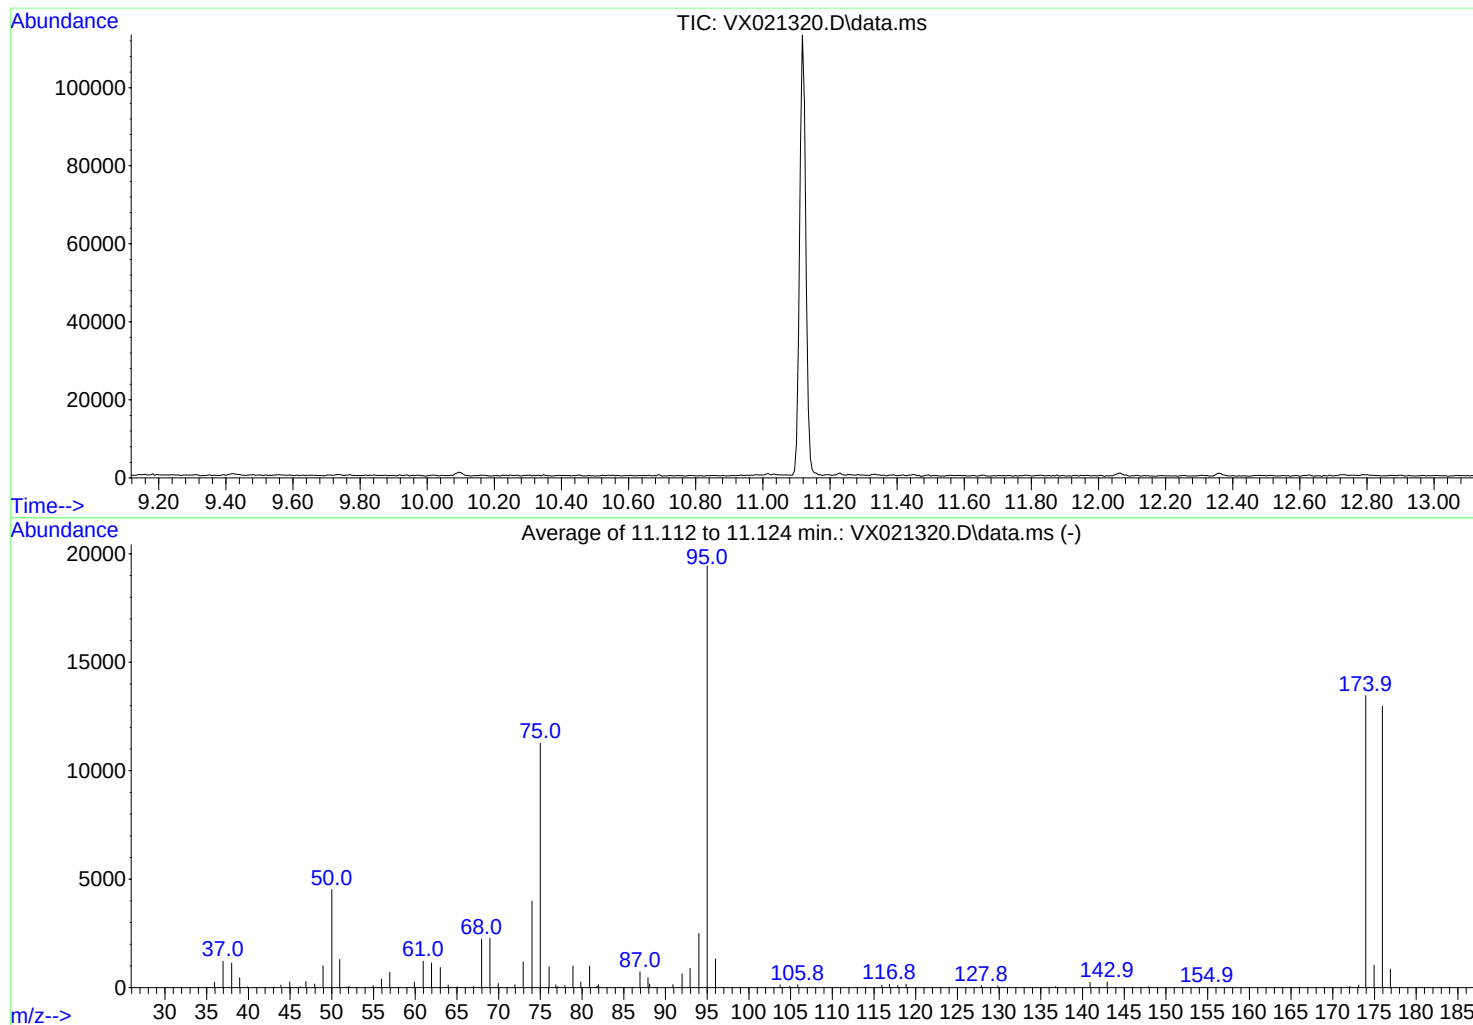

AutoFind: Scans 1704, 1705, 1706; Background Corrected with Scan 1698

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.3	4524	PASS
75	95	30	60	58.0	11269	PASS
95	95	100	100	100.0	19445	PASS
96	95	5	9	6.8	1320	PASS
173	174	0.00	2	0.9	120	PASS
174	95	50	100	69.2	13463	PASS
175	174	5	9	7.7	1034	PASS
176	174	95	101	96.4	12978	PASS
177	176	5	9	6.6	856	PASS