

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032123\
 Data File : VX034645.D
 Acq On : 21 Mar 2023 09:45
 Operator : JC/MD
 Sample : VX0321MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0321MBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
 Title : SW846 8260

Signal : TIC: VX034645.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.581	70	81	83	rBV4	12094	30979	2.16%	0.385%
2	5.379	692	704	720	rBV2	180065	535109	37.38%	6.653%
3	5.544	720	731	752	rVB	326505	931090	65.04%	11.576%
4	5.952	787	798	815	rBV	212320	571263	39.90%	7.102%
5	6.757	920	930	943	rBV	503927	1208411	84.41%	15.024%
6	8.647	1233	1240	1251	rBV	915661	1431607	100.00%	17.799%
7	10.055	1465	1471	1489	rBV	860285	1229934	85.91%	15.291%
8	11.079	1634	1639	1650	rBV	735082	944890	66.00%	11.748%
9	12.018	1788	1793	1808	rVB	871912	1136075	79.36%	14.125%
10	13.725	2069	2073	2077	rBV2	18915	23926	1.67%	0.297%




Sum of corrected areas: 8043284

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032123\
Data File : VX034645.D
Acq On : 21 Mar 2023 09:45
Operator : JC/MD
Sample : VX0321MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0321MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

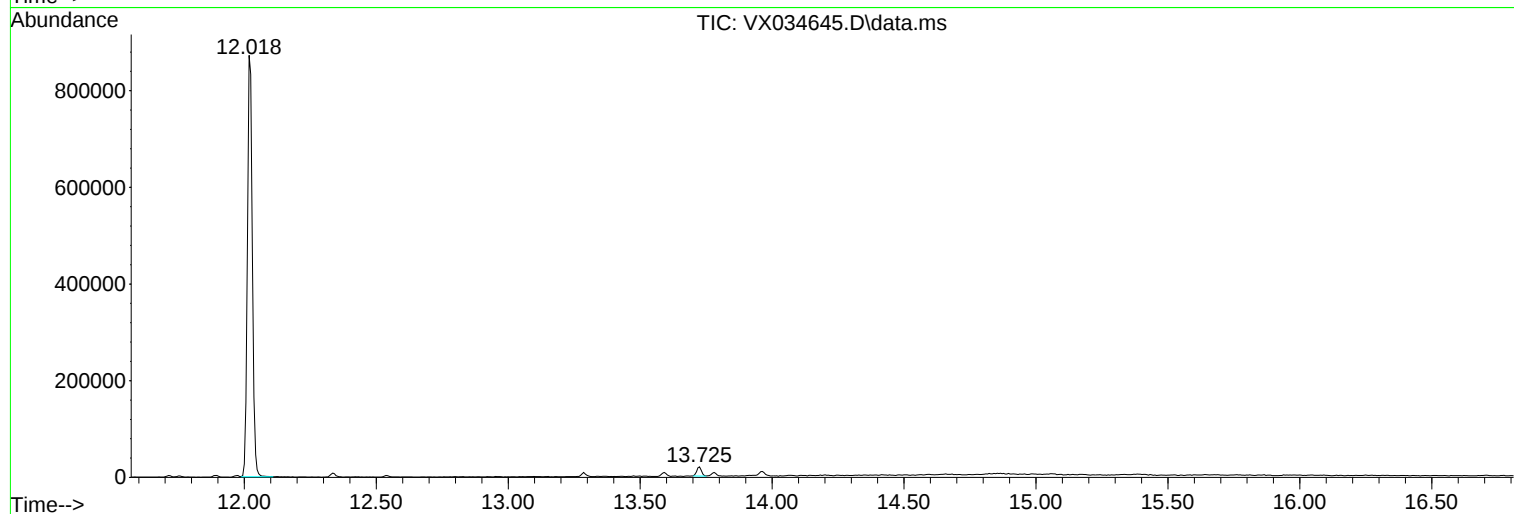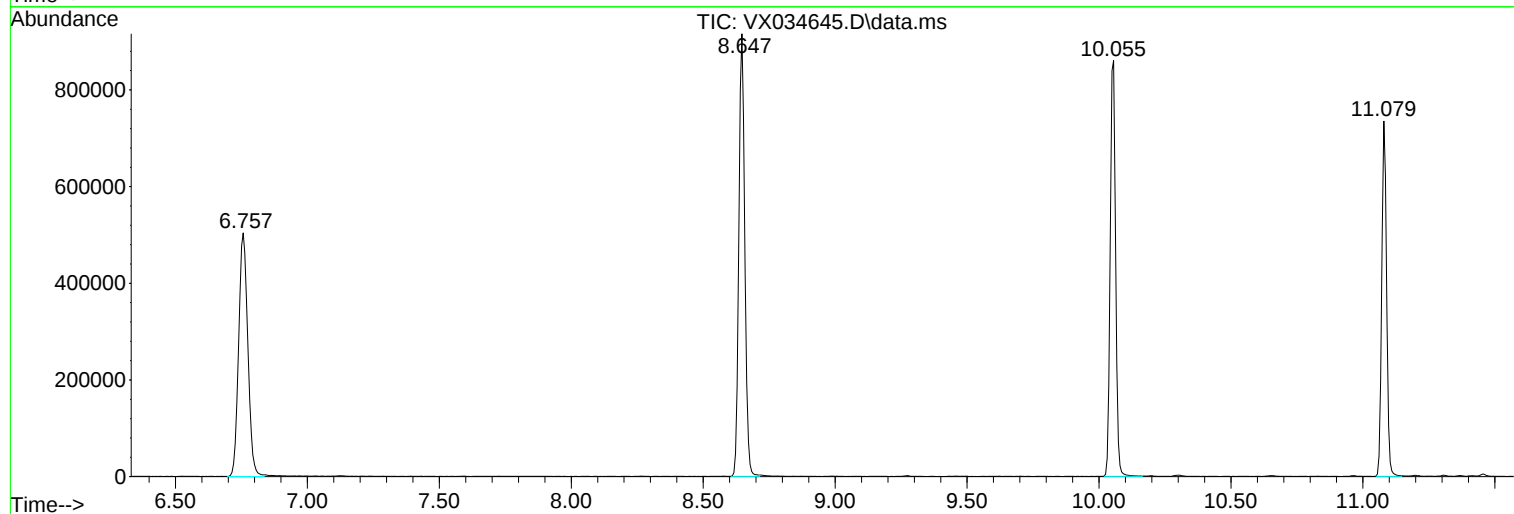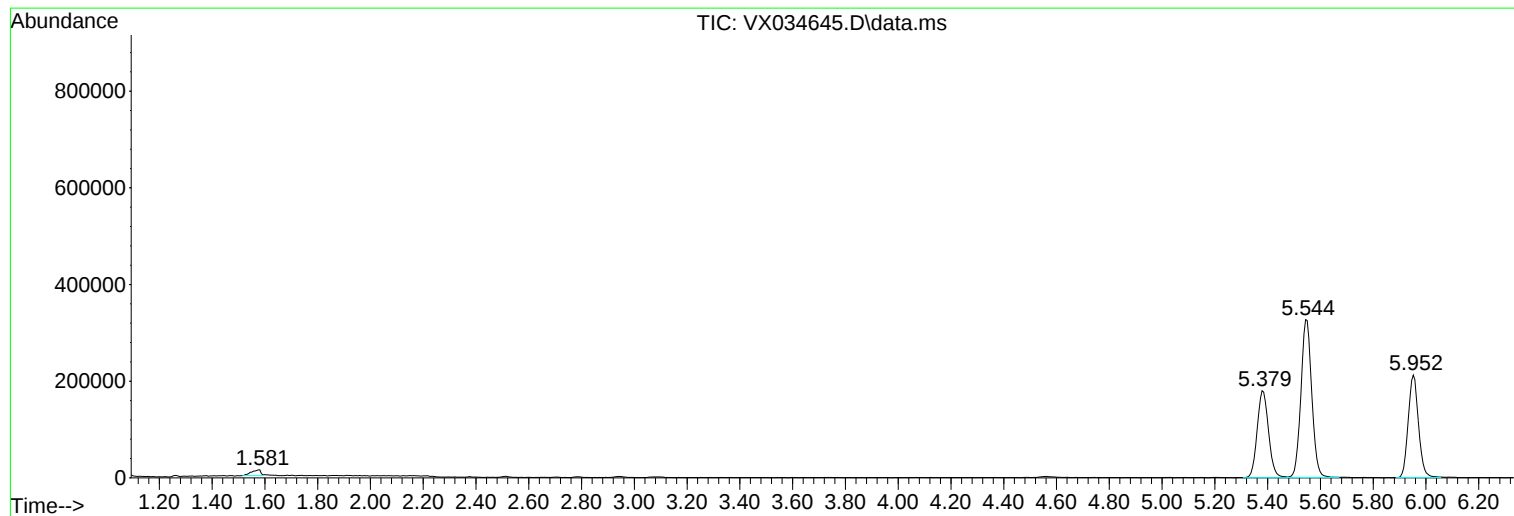

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032123\
Data File : VX034645.D
Acq On : 21 Mar 2023 09:45
Operator : JC/MD
Sample : VX0321MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0321MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032123\
Data File : VX034645.D
Acq On : 21 Mar 2023 09:45
Operator : JC/MD
Sample : VX0321MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0321MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc