

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX032123\  
 Data File : VX034646.D  
 Acq On : 21 Mar 2023 10:09  
 Operator : JC/MD  
 Sample : VX0321WBL01  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VX0321WBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031023W.M

Title : SW846 8260

Signal : TIC: VX034646.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.557       | 68            | 77          | 84           | rBV3     | 8508           | 20418         | 1.34%           | 0.274%        |
| 2         | 5.385       | 694           | 705         | 721          | rBV2     | 146138         | 432883        | 28.33%          | 5.813%        |
| 3         | 5.550       | 721           | 732         | 749          | rVB      | 260345         | 736573        | 48.20%          | 9.890%        |
| 4         | 5.952       | 787           | 798         | 815          | rBV      | 172120         | 466609        | 30.53%          | 6.265%        |
| 5         | 6.757       | 920           | 930         | 947          | rBV      | 405833         | 980465        | 64.16%          | 13.165%       |
| 6         | 8.647       | 1233          | 1240        | 1257         | rBV      | 988032         | 1528189       | 100.00%         | 20.520%       |
| 7         | 10.055      | 1465          | 1471        | 1487         | rBV      | 938712         | 1331103       | 87.10%          | 17.874%       |
| 8         | 11.079      | 1634          | 1639        | 1650         | rBV      | 739736         | 913978        | 59.81%          | 12.273%       |
| 9         | 12.018      | 1788          | 1793        | 1804         | rBV      | 789842         | 1037137       | 67.87%          | 13.926%       |




Sum of corrected areas: 7447355

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX032123\  
Data File : VX034646.D  
Acq On : 21 Mar 2023 10:09  
Operator : JC/MD  
Sample : VX0321WBL01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX0321WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031023W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

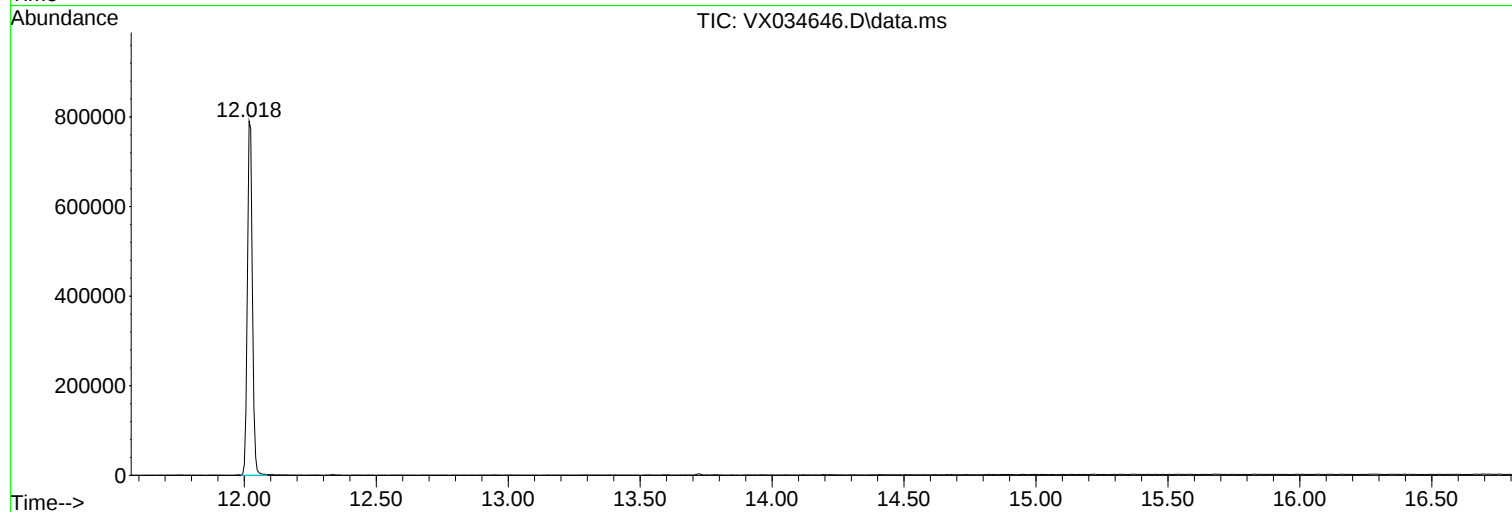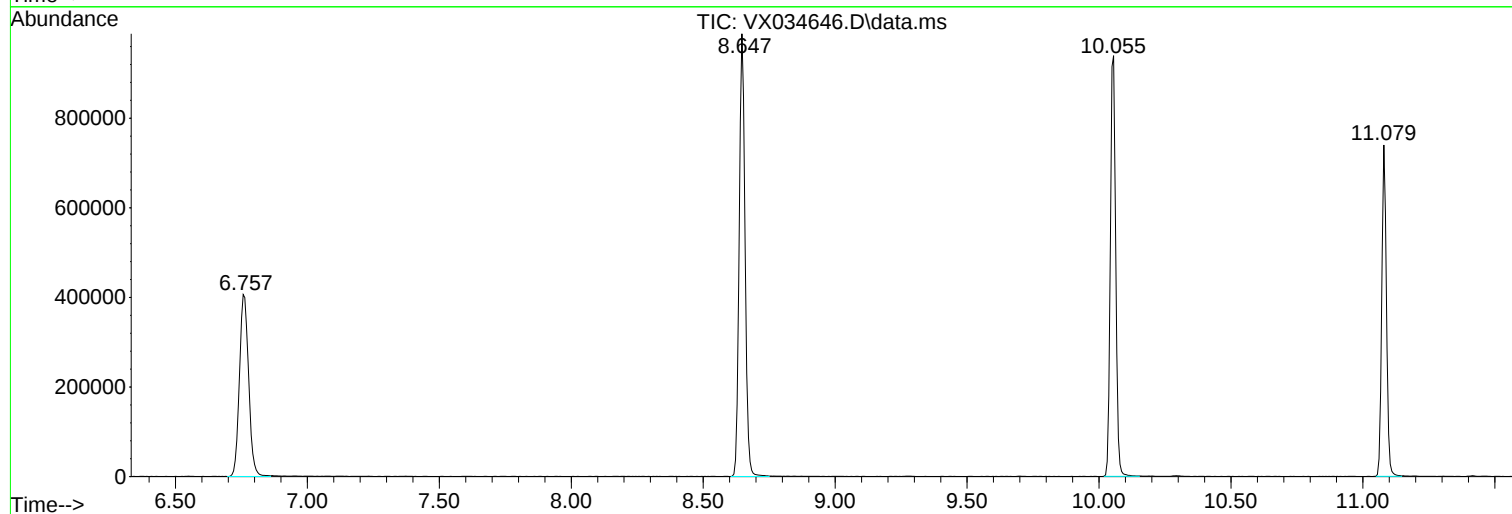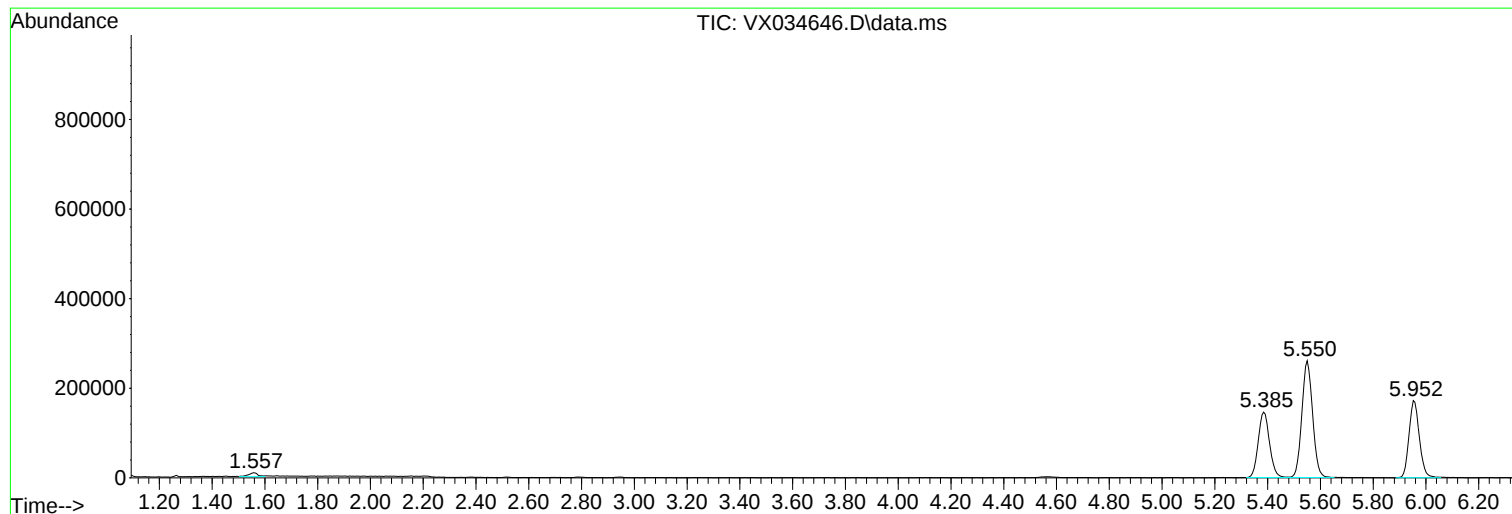

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX032123\  
Data File : VX034646.D  
Acq On : 21 Mar 2023 10:09  
Operator : JC/MD  
Sample : VX0321WBL01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX0321WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031023W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX032123\  
Data File : VX034646.D  
Acq On : 21 Mar 2023 10:09  
Operator : JC/MD  
Sample : VX0321WBL01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX0321WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031023W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|