

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032123\
 Data File : VX034656.D
 Acq On : 21 Mar 2023 15:50
 Operator : JC/MD
 Sample : 01946-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 NWB-1896

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M

Title : SW846 8260

Signal : TIC: VX034656.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	32	rBV	18799	28732	2.13%	0.325%
2	1.575	67	80	81	rBV6	19048	53602	3.97%	0.606%
3	1.624	84	88	101	rVV	99791	188742	13.99%	2.134%
4	2.441	217	222	237	rVV	29904	82573	6.12%	0.934%
5	2.733	261	270	293	rBV	251207	591029	43.79%	6.682%
6	3.416	377	382	392	rVB4	8140	23795	1.76%	0.269%
7	5.318	684	694	696	rBV2	7591	16688	1.24%	0.189%
8	5.391	696	706	720	rVV	89658	342208	25.36%	3.869%
9	5.538	720	730	748	rVB	268038	789046	58.47%	8.920%
10	5.952	786	798	817	rBV	157075	474920	35.19%	5.369%
11	6.757	919	930	949	rBV	407604	1011710	74.97%	11.438%
12	8.647	1233	1240	1259	rBV	834641	1349538	100.00%	15.257%
13	10.055	1465	1471	1493	rBV	786419	1163451	86.21%	13.153%
14	11.085	1634	1640	1651	rBV	646263	955310	70.79%	10.800%
15	12.024	1788	1794	1804	rBV	903345	1166798	86.46%	13.191%
16	14.993	2274	2281	2303	rBV	353105	607189	44.99%	6.865%




Sum of corrected areas: 8845331

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032123\
Data File : VX034656.D
Acq On : 21 Mar 2023 15:50
Operator : JC/MD
Sample : 01946-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
NWB-1896

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

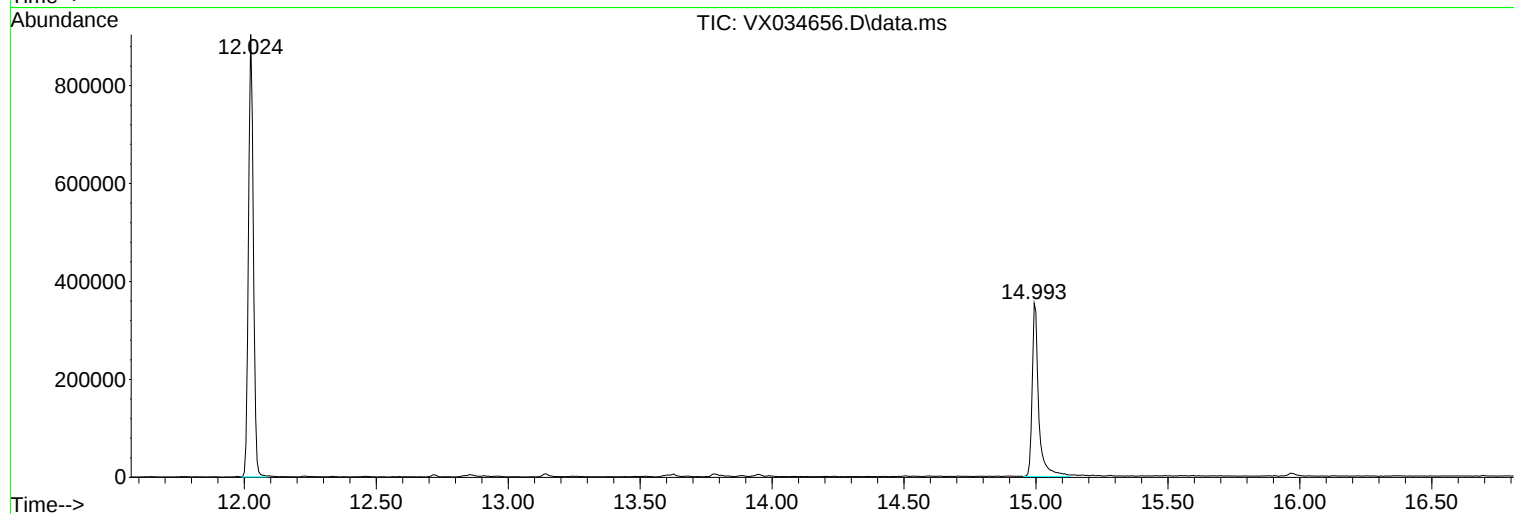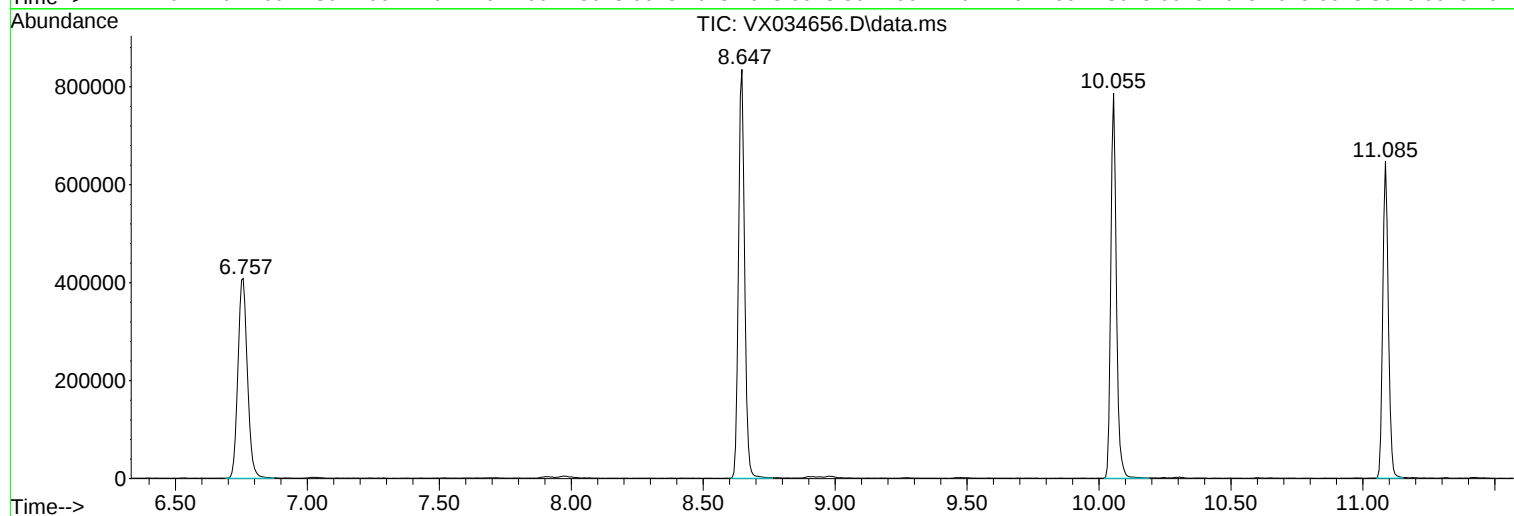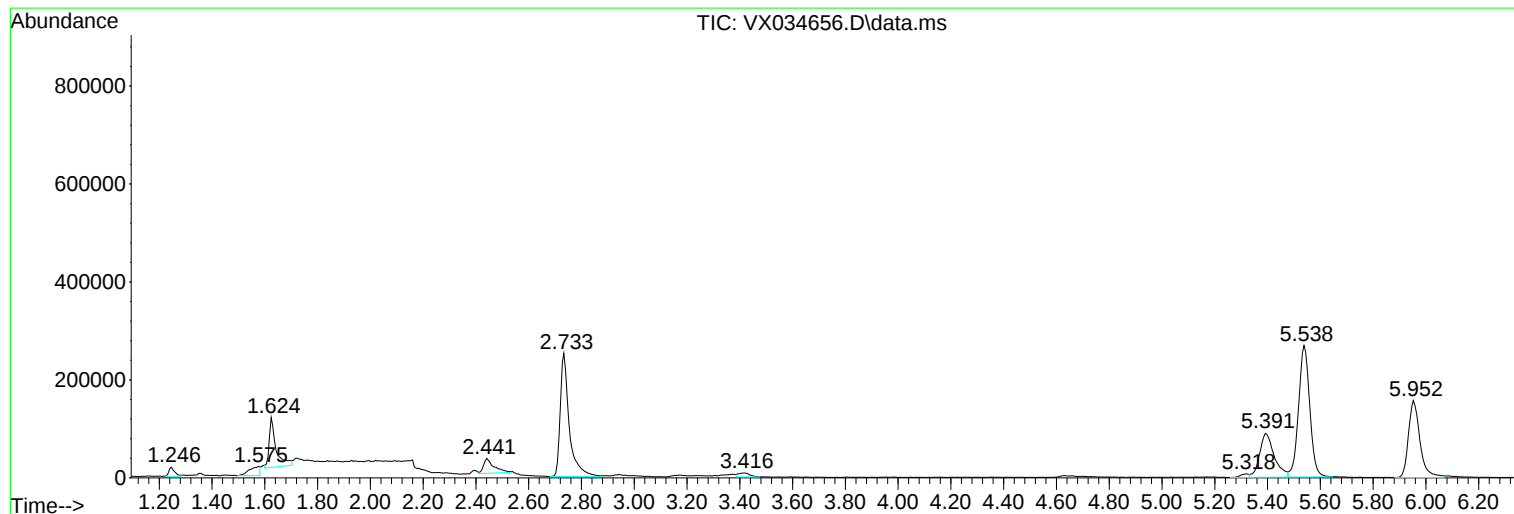

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032123\
Data File : VX034656.D
Acq On : 21 Mar 2023 15:50
Operator : JC/MD
Sample : 01946-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
NWB-1896










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown14.993 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.993	26.02 ug/l	607189	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopenten-4-one, 1,2,3,3-tetra...	138	C9H14O	1000163-38-6	42
2			(2Z,4E)-3,7-Dimethyl-2,4-octadiene	138	C10H18	1000374-08-4	30
3			trans-3,5-Dimethylcyclohexene	110	C8H14	056021-63-7	25
4			3,5-Dodecadiene, 2-methyl-	180	C13H24	055638-51-2	25
5			2-(2-Hydroxycycloheptyl)-furan	180	C11H16O2	1000145-02-9	20

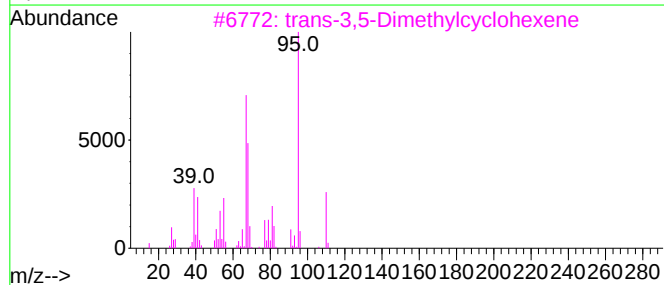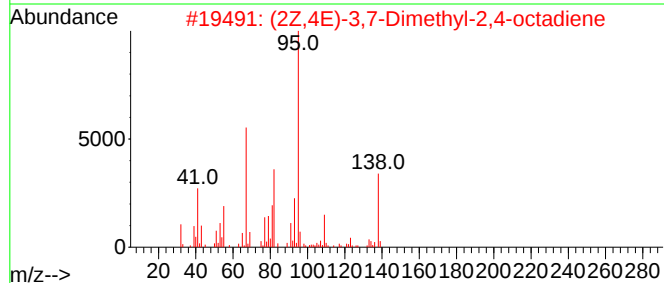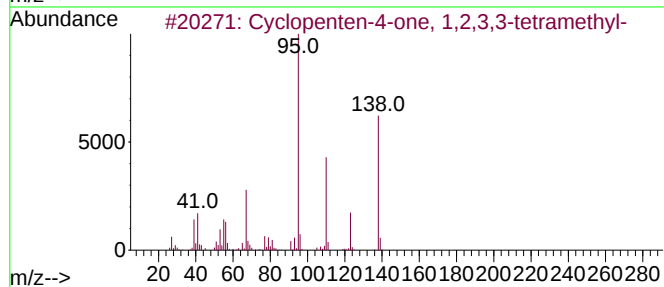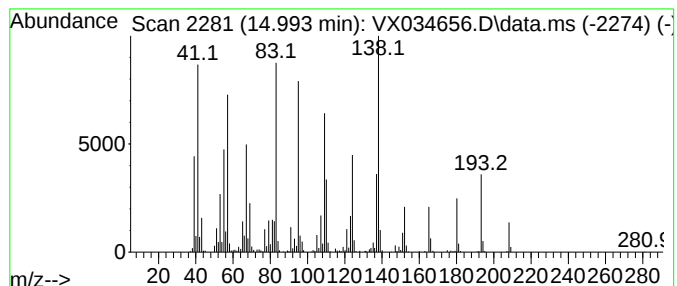

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032123\
Data File : VX034656.D
Acq On : 21 Mar 2023 15:50
Operator : JC/MD
Sample : 01946-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
NWB-1896

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown14.993	14.993	26.0	ug/l	607189	4	12.024	1166800	50.0