



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032123\
Data File : VX034643.D
Acq On : 21 Mar 2023 08:45
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Title : SW846 8260
Last Update : Mon Mar 13 10:29:32 2023

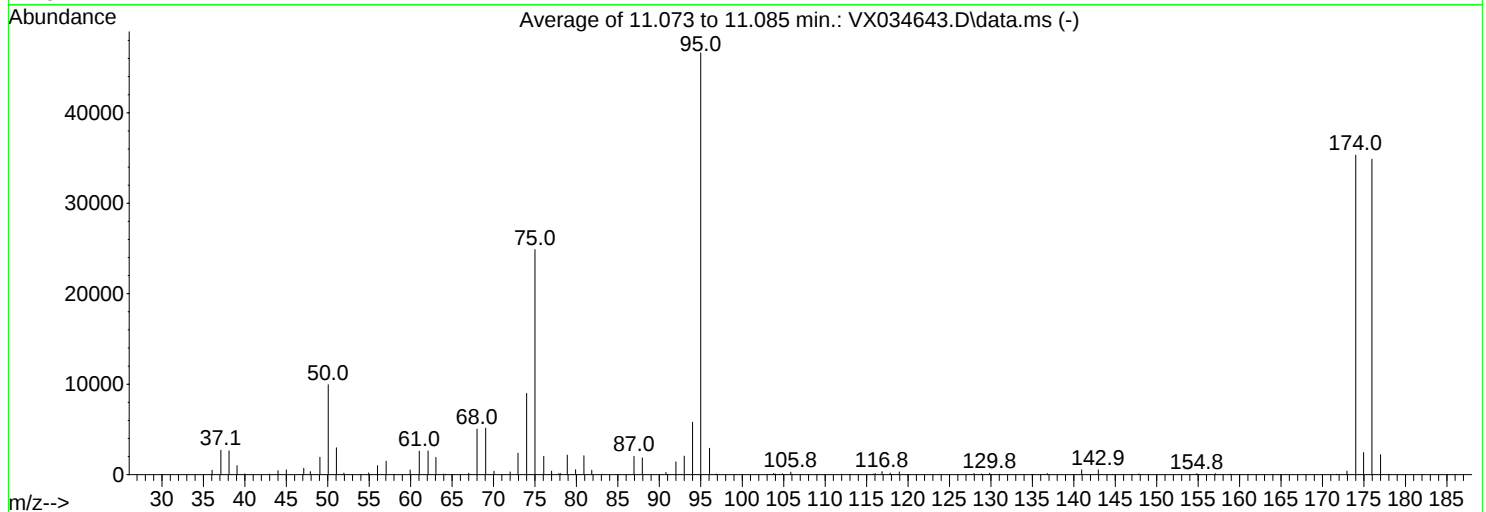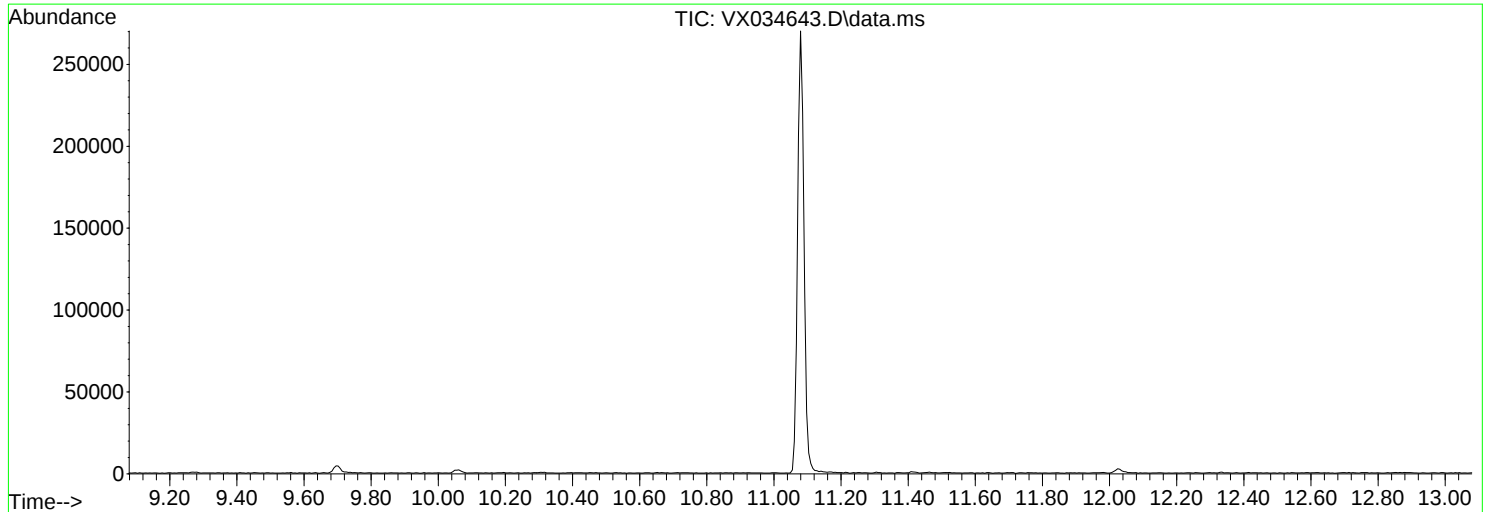

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.3	9938	PASS
75	95	30	60	53.4	24880	PASS
95	95	100	100	100.0	46629	PASS
96	95	5	9	6.3	2922	PASS
173	174	0.00	2	1.1	384	PASS
174	95	50	100	75.7	35317	PASS
175	174	5	9	6.9	2447	PASS
176	174	95	101	98.8	34877	PASS
177	176	5	9	6.3	2211	PASS