


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX032219\
Data File : VX008329.D
Acq On : 22 Mar 2019 09:39
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102418W.M
Title : SW846 8260
Last Update : Thu Oct 25 02:52:45 2018

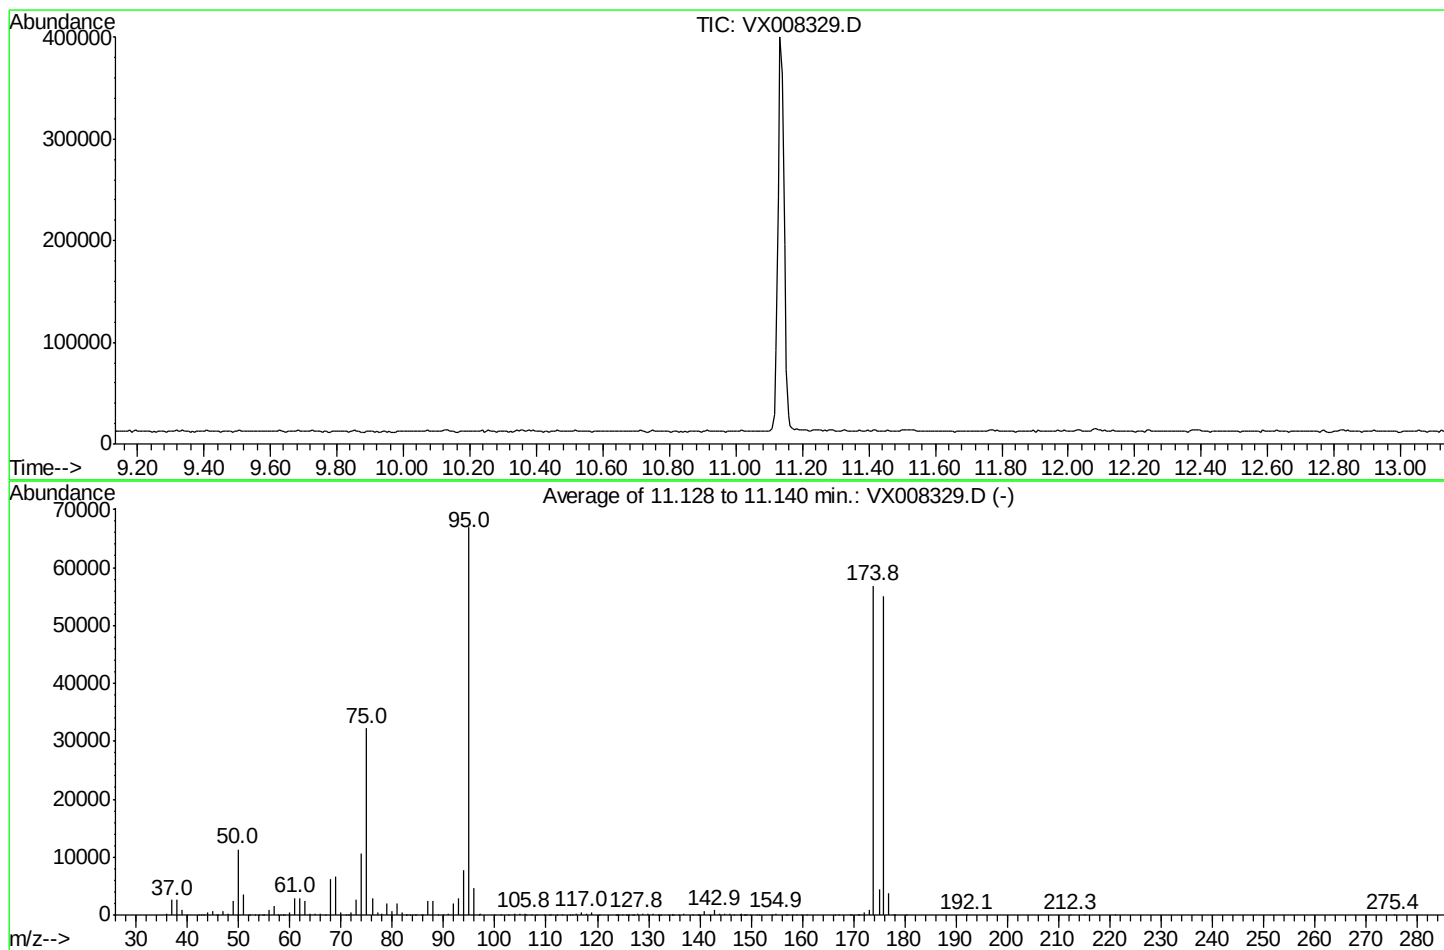

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1628

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	11345	PASS
75	95	30	60	48.2	32239	PASS
95	95	100	100	100.0	66933	PASS
96	95	5	9	7.0	4687	PASS
173	174	0.00	2	1.7	968	PASS
174	95	50	100	84.9	56846	PASS
175	174	5	9	7.8	4455	PASS
176	174	95	101	96.9	55090	PASS
177	176	5	9	6.7	3713	PASS