

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032221\
 Data File : VX021362.D
 Acq On : 22 Mar 2021 16:42
 Operator : JC/MD
 Sample : M1736-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP02-20210317

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M

Title : SW846 8260

Signal : TIC: VX021362.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.593	77	86	90	rBV4	3553	7537	1.68%	0.302%
2	2.581	245	254	264	rBV	2709	6265	1.40%	0.251%
3	5.464	731	744	757	rBV	54549	153067	34.10%	6.130%
4	5.623	759	771	784	rBV2	89865	253511	56.47%	10.152%
5	6.029	829	840	856	rBV	62326	164625	36.67%	6.592%
6	6.829	964	976	988	rBV	140040	329005	73.29%	13.175%
7	7.188	1028	1037	1047	rBV3	71952	156888	34.95%	6.283%
8	8.694	1286	1293	1318	rBV	283405	448934	100.00%	17.978%
9	10.094	1525	1531	1548	rVB	274199	376897	83.95%	15.093%
10	11.118	1699	1705	1717	rVB	212883	282720	62.98%	11.322%
11	12.059	1860	1865	1873	rVB	262018	317710	70.77%	12.723%




Sum of corrected areas: 2497159

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032221\
Data File : VX021362.D
Acq On : 22 Mar 2021 16:42
Operator : JC/MD
Sample : M1736-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP02-20210317

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

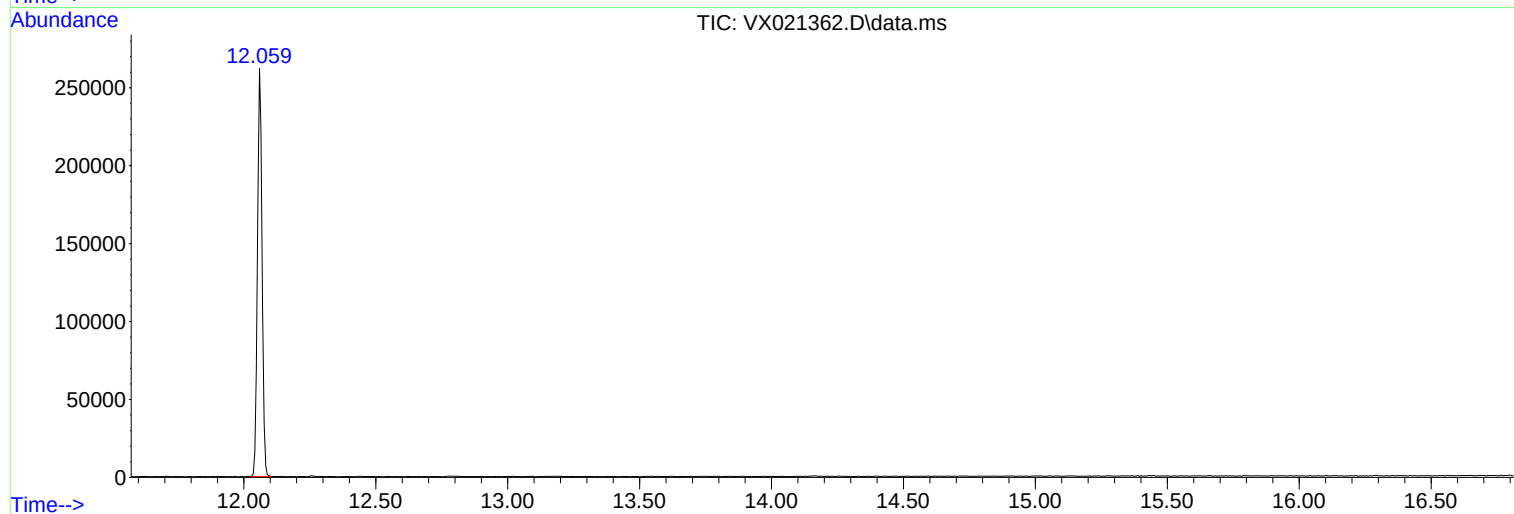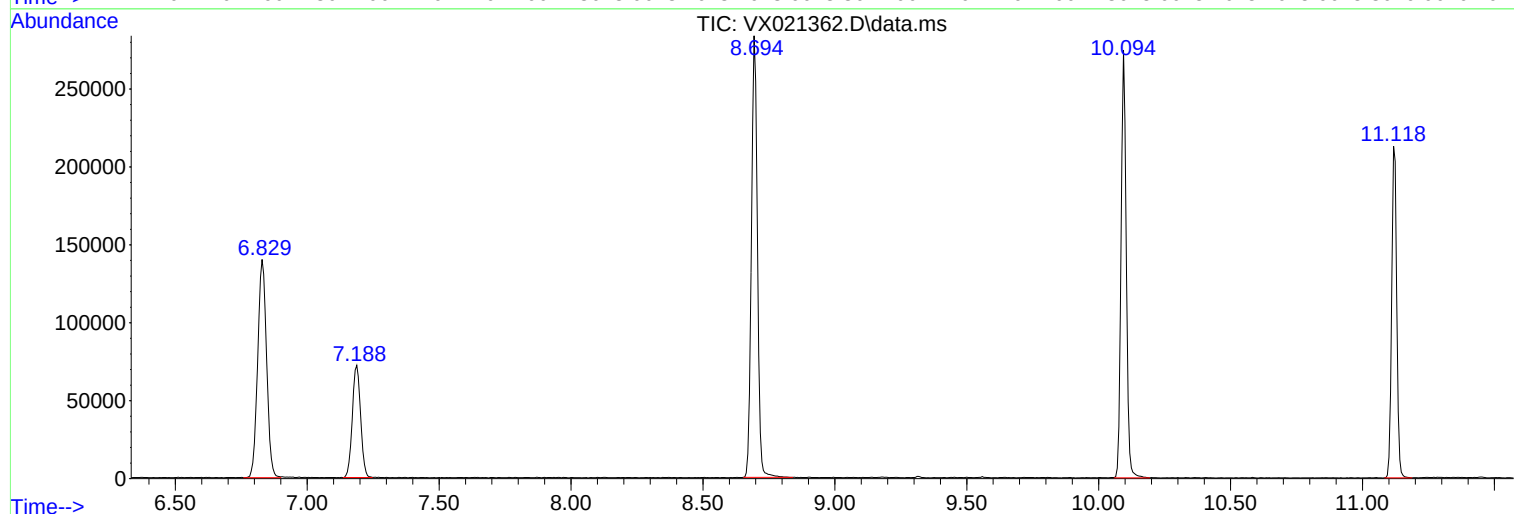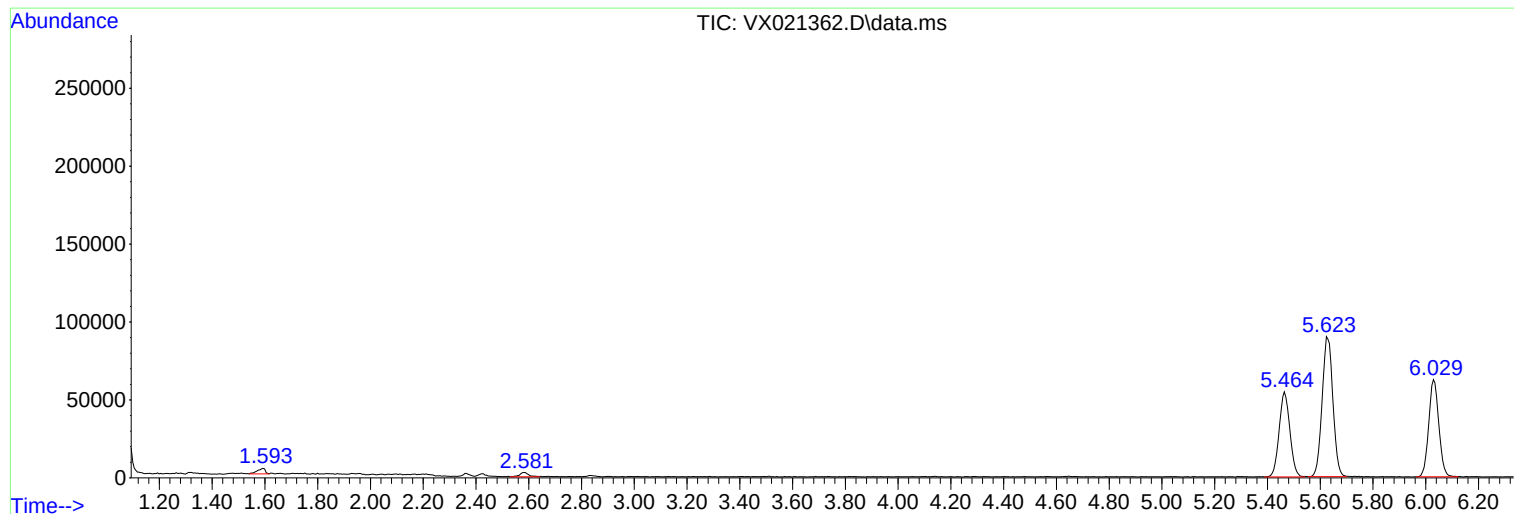

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032221\
Data File : VX021362.D
Acq On : 22 Mar 2021 16:42
Operator : JC/MD
Sample : M1736-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP02-20210317

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032221\
Data File : VX021362.D
Acq On : 22 Mar 2021 16:42
Operator : JC/MD
Sample : M1736-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP02-20210317

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
