
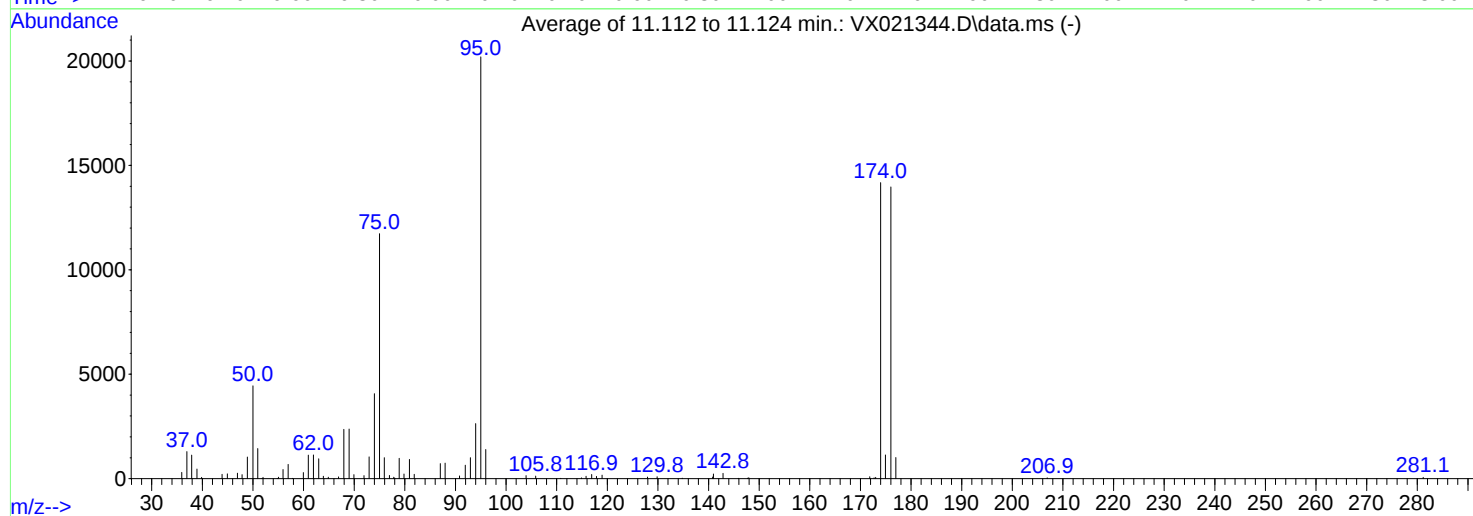


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032221\
Data File : VX021344.D
Acq On : 22 Mar 2021 09:23
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Title : SW846 8260
Last Update : Tue Mar 16 14:00:21 2021

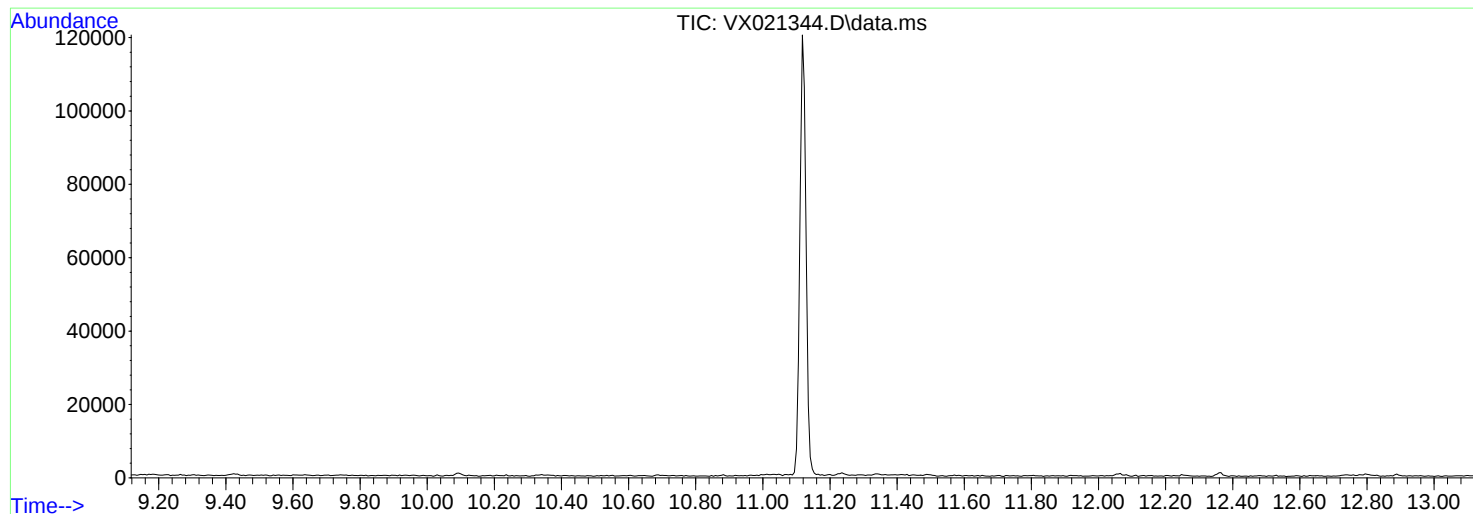

AutoFind: Scans 1704, 1705, 1706; Background Corrected with Scan 1698

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	4444	PASS
75	95	30	60	58.1	11731	PASS
95	95	100	100	100.0	20199	PASS
96	95	5	9	6.9	1394	PASS
173	174	0.00	2	0.4	60	PASS
174	95	50	100	70.2	14176	PASS
175	174	5	9	8.0	1132	PASS
176	174	95	101	98.5	13966	PASS
177	176	5	9	7.3	1014	PASS