

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032222\
 Data File : VX027621.D
 Acq On : 22 Mar 2022 17:51
 Operator : JC/MD
 Sample : N1998-19
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP031622

Manual Integrations
 APPROVED

Reviewed By : John Carlone 03/24/2022
 Supervised By : Mahesh Dadoda 03/24/2022

Quant Time: Mar 23 01:49:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 17 15:02:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	355912	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	568065	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	520838	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	249685	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	188523	42.998	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	86.000%		
35) Dibromofluoromethane	5.391	113	181641	49.699	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	99.400%		
50) Toluene-d8	8.653	98	674025	48.735	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	97.480%		
62) 4-Bromofluorobenzene	11.079	95	246119	48.416	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	96.840%		
Target Compounds					Qvalue	
11) Tert butyl alcohol	2.965	59	36734	43.961	ug/l	99
16) Acetone	2.380	43	33766	18.894	ug/l	95
17) Carbon Disulfide	2.514	76	5475	0.651	ug/l #	94
19) Methyl tert-butyl Ether	3.117	73	117502	10.538	ug/l #	44
22) Diisopropyl ether	3.776	45	4606	0.456	ug/l #	69
25) 2-Butanone	4.568	43	11572	4.304	ug/l #	87
31) Cyclohexane	5.477	56	108840	19.991	ug/l	99
39) Methylcyclohexane	7.379	83	172218	27.420	ug/l	94
40) Benzene	6.044	78	724284	50.547	ug/l	98
42) 1,2-Dichloroethane	6.092	62	13576	2.528	ug/l	96
51) 4-Methyl-2-Pentanone	8.580	43	11282	2.207	ug/l	90
52) Toluene	8.720	92	1830848	190.671	ug/l	98
59) 2-Hexanone	9.439	43	27391	6.956	ug/l	67
64) Tetrachloroethene	9.275	164	1260	0.311	ug/l #	87
67) Ethyl Benzene	10.201	91	8699048	474.348	ug/l #	82
68) m/p-Xylenes	10.311	106	7433493	1029.451	ug/l	77
69) o-Xylene	10.647	106	2271469	323.985	ug/l	93
73) Isopropylbenzene	10.964	105	249930	13.743	ug/l	99
78) n-propylbenzene	11.305	91	1077940	53.994	ug/l	97
80) 1,3,5-Trimethylbenzene	11.457	105	3357040	219.320	ug/l	97
83) tert-Butylbenzene	11.719	119	177861	11.730	ug/l	88
84) 1,2,4-Trimethylbenzene	11.756	105	6126511	401.342	ug/l	93
85) sec-Butylbenzene	11.890	105	37378m	2.040	ug/l	
86) p-Isopropyltoluene	12.012	119	17704m	1.125	ug/l	
91) 1,2-Dichlorobenzene	12.341	146	3091	0.373	ug/l #	60
95) Naphthalene	13.780	128	2298478	132.830	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032222\
Data File : VX027621.D
Acq On : 22 Mar 2022 17:51
Operator : JC/MD
Sample : N1998-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1


Instrument :
MSVOA_X
ClientSampleId :
DUP031622

Quant Time: Mar 23 01:49:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260
QLast Update : Thu Mar 17 15:02:59 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : John Carlone 03/24/2022
Supervised By : Mahesh Dadoda 03/24/2022

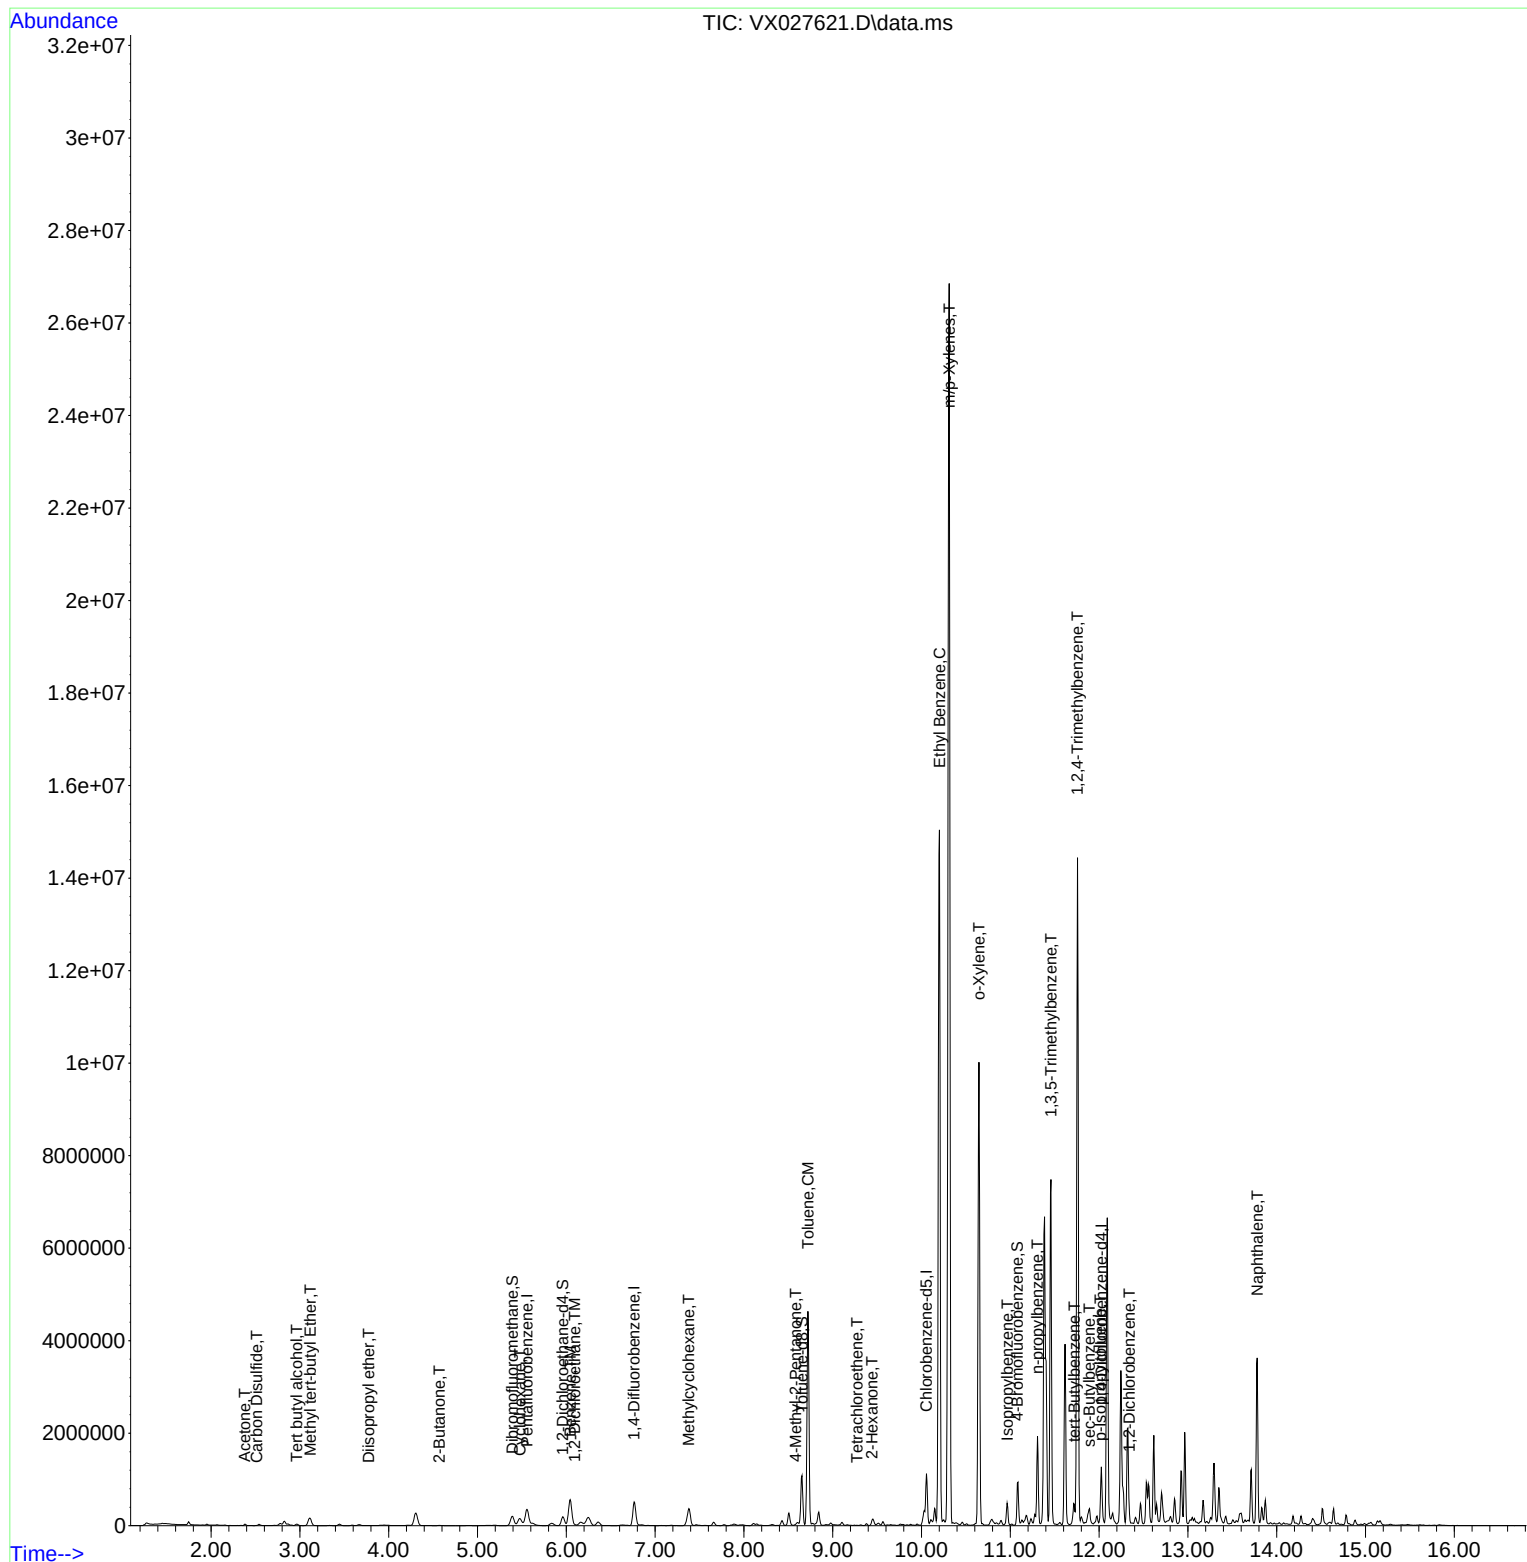

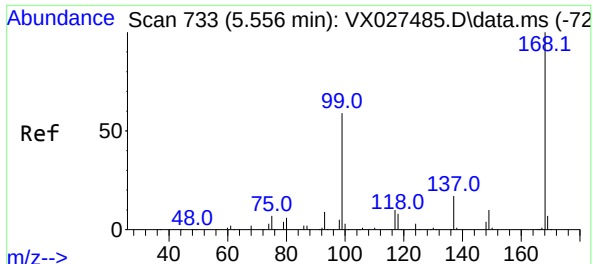

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51




Instrument :
MSVOA_X
ClientSampleId :
DUP031622




Tgt Ion:168 Resp: 35591
Ion Ratio Lower Upper
168 100
99 53.9 41.7 62.5

Manual Integrations
APPROVED



Reviewed By :John Carlone 03/24/2022
Supervised By :Mahesh Dadoda 03/24/2022

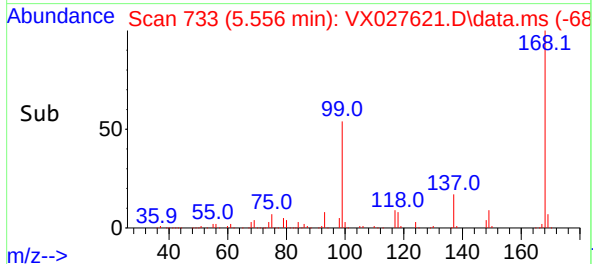


#11
Tert butyl alcohol
Concen: 43.961 ug/l
RT: 2.965 min Scan# 308
Delta R.T. -0.006 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51

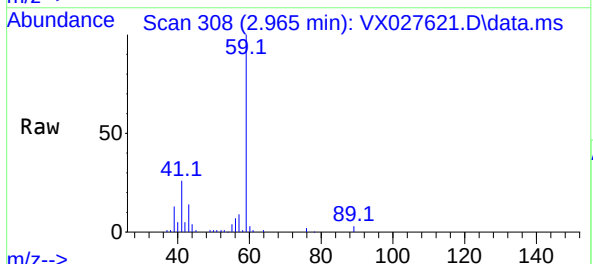


Tgt Ion: 59 Resp: 36734
Ion Ratio Lower Upper
59 100
57 10.1 8.3 12.5

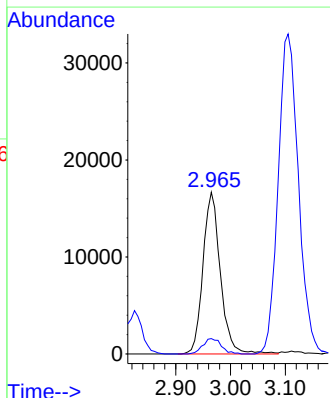



#16
Acetone
Concen: 18.894 ug/l
RT: 2.380 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51




Instrument :
MSVOA_X
ClientSampleId :
DUP031622



Tgt Ion: 43 Resp: 33760
Ion Ratio Lower Upper
43 100
58 33.0 28.8 43.2




Manual Integrations
APPROVED


Reviewed By :John Carlone 03/24/2022
Supervised By :Mahesh Dadoda 03/24/2022

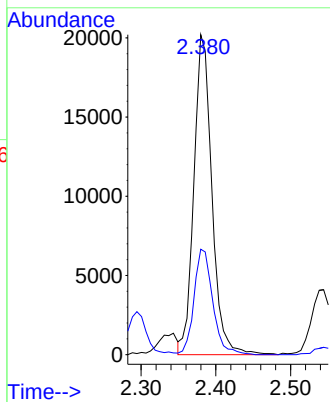

#17
Carbon Disulfide
Concen: 0.651 ug/l
RT: 2.514 min Scan# 234
Delta R.T. 0.006 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51


Tgt Ion: 76 Resp: 5475
Ion Ratio Lower Upper
76 100
78 6.7 7.2 10.8#

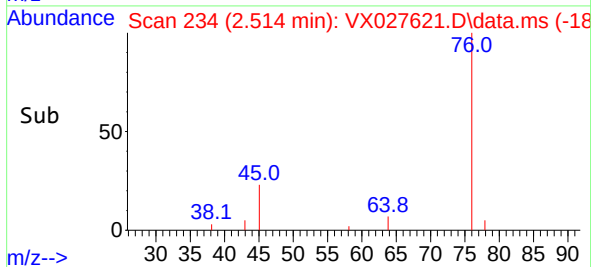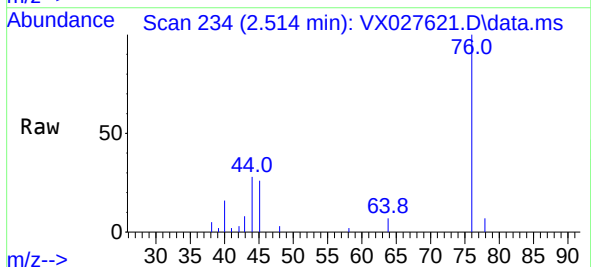



#19
Methyl tert-butyl Ether
Concen: 10.538 ug/l
RT: 3.117 min Scan# 311
Delta R.T. 0.000 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51




Instrument :
MSVOA_X
ClientSampleId :
DUP031622



Tgt Ion: 73 Resp: 117502
Ion Ratio Lower Upper
73 100
57 47.1 16.8 25.2




Manual Integrations
APPROVED


Reviewed By :John Carlone 03/24/2022
Supervised By :Mahesh Dadoda 03/24/2022

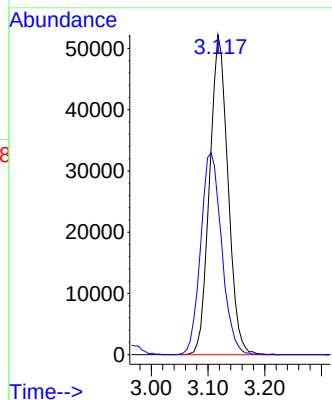

#22
Diisopropyl ether
Concen: 0.456 ug/l
RT: 3.776 min Scan# 441
Delta R.T. 0.012 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51


Tgt Ion: 45 Resp: 4606
Ion Ratio Lower Upper
45 100
43 34.9 50.8 76.2#
87 19.8 26.6 39.8#
59 5.0 10.5 15.7#

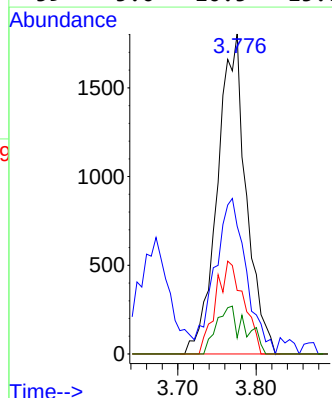



#25
2-Butanone
Concen: 4.304 ug/l
RT: 4.568 min Scan# 51
Delta R.T. 0.006 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51




Instrument :
MSVOA_X
ClientSampleId :
DUP031622



Tgt Ion: 43 Resp: 11572
Ion Ratio Lower Upper
43 100
72 23.5 24.4 36.6




Manual Integrations
APPROVED


Reviewed By :John Carlone 03/24/2022
Supervised By :Mahesh Dadoda 03/24/2022



#31
Cyclohexane
Concen: 19.991 ug/l
RT: 5.477 min Scan# 720
Delta R.T. 0.006 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51


Tgt Ion: 56 Resp: 108840
Ion Ratio Lower Upper
56 100
69 31.8 26.7 40.1
84 97.4 77.2 115.8

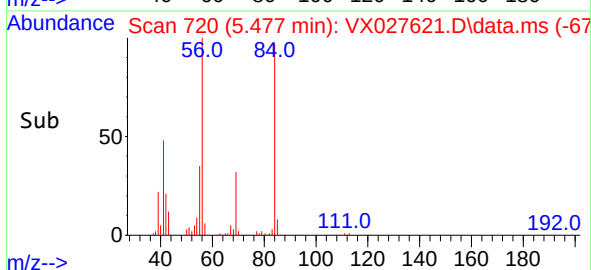



#33
1,2-Dichloroethane-d4
Concen: 42.998 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51




Instrument :
MSVOA_X
ClientSampleId :
DUP031622




Tgt Ion: 65 Resp: 18852
Ion Ratio Lower Upper
65 100
67 53.0 0.0 107.4

Manual Integrations
APPROVED



Reviewed By :John Carlone 03/24/2022
Supervised By :Mahesh Dadoda 03/24/2022




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 931
Delta R.T. 0.000 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51




Tgt Ion:114 Resp: 568065
Ion Ratio Lower Upper
114 100
63 18.3 0.0 36.8
88 15.9 0.0 32.4

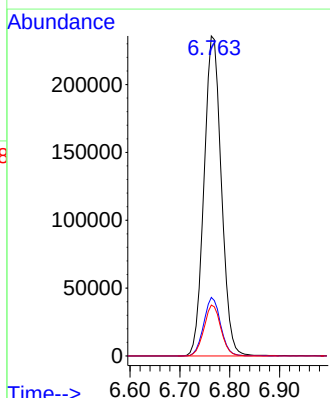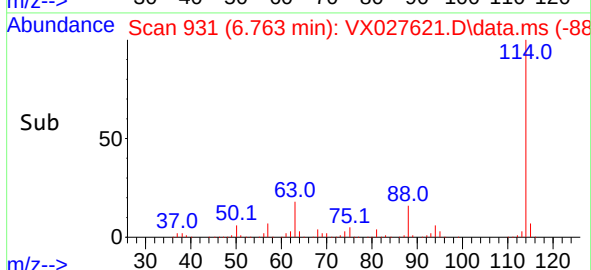

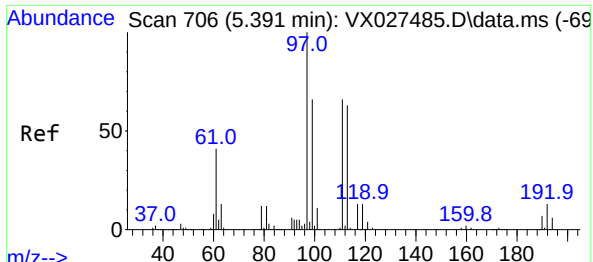

#35
Dibromofluoromethane
Concen: 49.699 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51




Instrument :
MSVOA_X
ClientSampleId :
DUP031622

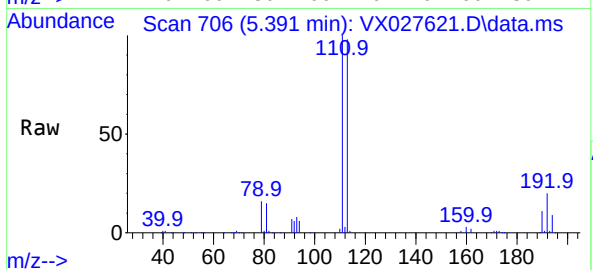

Tgt Ion:113 Resp: 18164
Ion Ratio Lower Upper
113 100
111 101.7 82.8 124.2
192 20.5 16.9 25.3




Manual Integrations
APPROVED


Reviewed By :John Carlone 03/24/2022
Supervised By :Mahesh Dadoda 03/24/2022

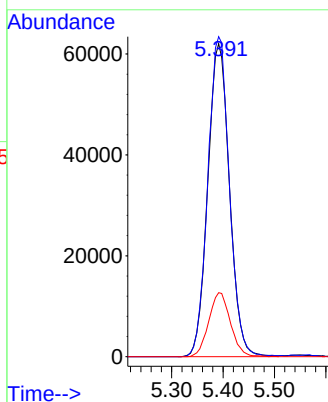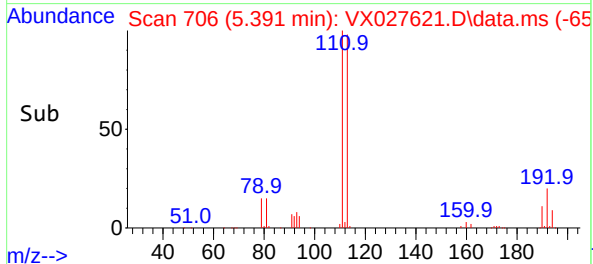

#39
Methylcyclohexane
Concen: 27.420 ug/l
RT: 7.379 min Scan# 1032
Delta R.T. -0.006 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51


Tgt Ion: 83 Resp: 172218
Ion Ratio Lower Upper
83 100
55 75.1 54.6 81.8
98 45.2 37.4 56.2

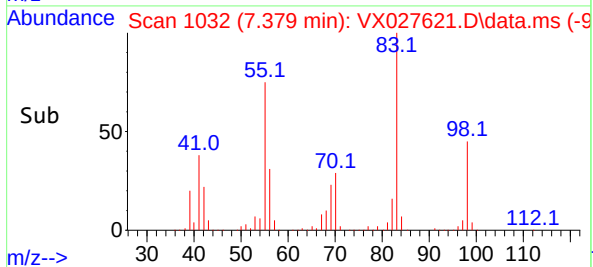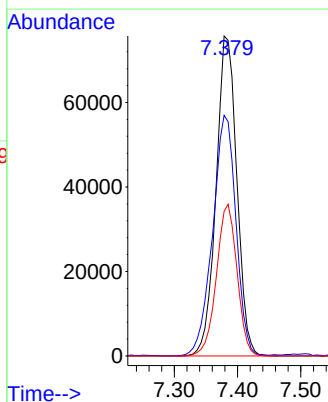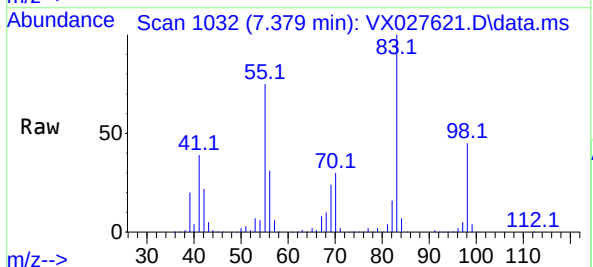



#40
Benzene
Concen: 50.547 ug/l
RT: 6.044 min Scan# 813
Delta R.T. 0.000 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51




Instrument :
MSVOA_X
ClientSampleId :
DUP031622



Tgt Ion: 78 Resp: 724284
Ion Ratio Lower Upper
78 100
77 23.1 19.3 28.9




Manual Integrations
APPROVED


Reviewed By :John Carlone 03/24/2022
Supervised By :Mahesh Dadoda 03/24/2022



#42
1,2-Dichloroethane
Concen: 2.528 ug/l
RT: 6.092 min Scan# 821
Delta R.T. 0.000 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51


Tgt Ion: 62 Resp: 13576
Ion Ratio Lower Upper
62 100
98 11.7 0.0 20.4

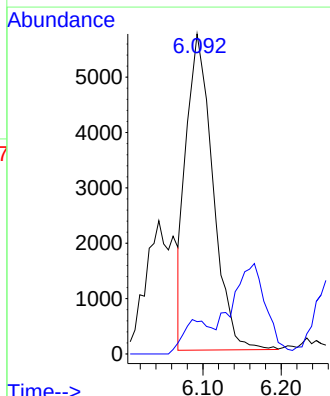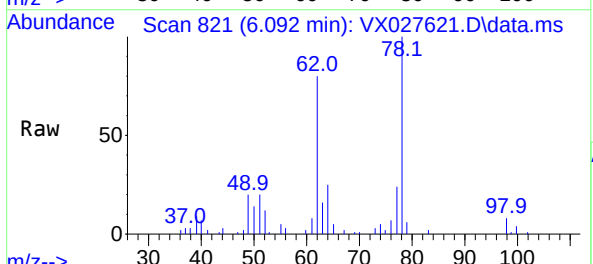



#50
Toluene-d8
Concen: 48.735 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.000 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51




Instrument :
MSVOA_X
ClientSampleId :
DUP031622




Tgt Ion: 98 Resp: 674025
Ion Ratio Lower Upper
98 100
100 64.1 52.6 78.8

Manual Integrations
APPROVED



Reviewed By :John Carlone 03/24/2022
Supervised By :Mahesh Dadoda 03/24/2022

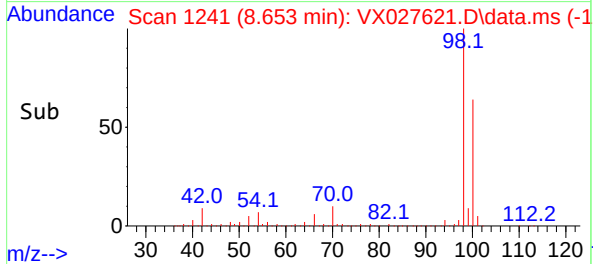


#51
4-Methyl-2-Pentanone
Concen: 2.207 ug/l
RT: 8.580 min Scan# 1229
Delta R.T. 0.000 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51

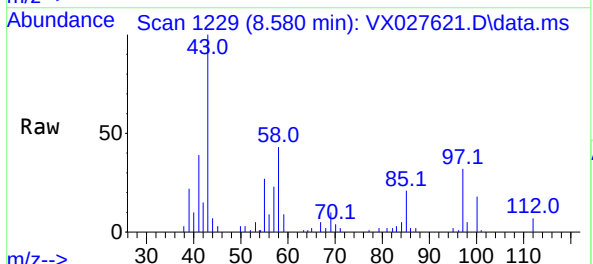


Tgt Ion: 43 Resp: 11282
Ion Ratio Lower Upper
43 100
58 38.7 36.1 54.1

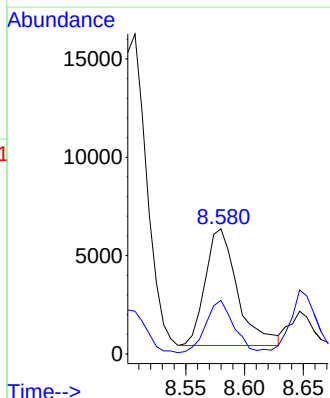



#52
Toluene
Concen: 190.671 ug/l
RT: 8.720 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51




Instrument :
MSVOA_X
ClientSampleId :
DUP031622




Tgt Ion: 92 Resp: 183084
Ion Ratio Lower Upper
92 100
91 168.8 137.5 206.3

Manual Integrations
APPROVED



Reviewed By :John Carlone 03/24/2022
Supervised By :Mahesh Dadoda 03/24/2022

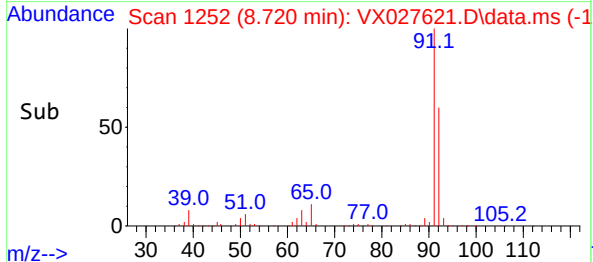


#59
2-Hexanone
Concen: 6.956 ug/l
RT: 9.439 min Scan# 1370
Delta R.T. 0.006 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51

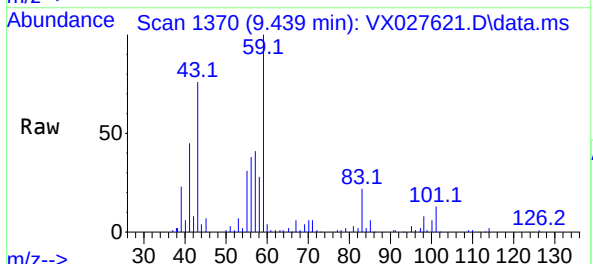


Tgt Ion: 43 Resp: 27391
Ion Ratio Lower Upper
43 100
58 38.4 31.9 95.7

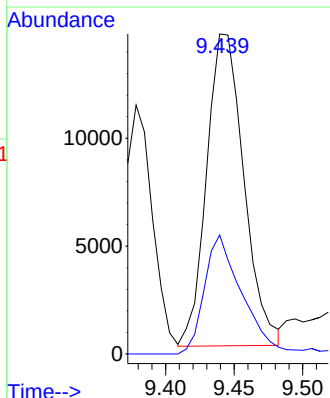



#62
4-Bromofluorobenzene
Concen: 48.416 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.006 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51




Instrument :
MSVOA_X
ClientSampleId :
DUP031622




Tgt Ion: 95 Resp: 246119
Ion Ratio Lower Upper
95 100
174 81.6 0.0 163.0
176 78.4 0.0 155.0

Manual Integrations
APPROVED



Reviewed By :John Carlone 03/24/2022
Supervised By :Mahesh Dadoda 03/24/2022

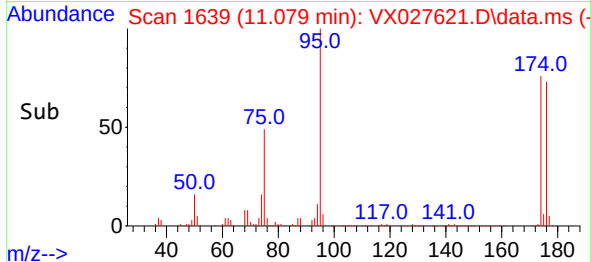


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51




Tgt Ion:117 Resp: 520838
Ion Ratio Lower Upper
117 100
82 54.3 41.8 62.8
119 32.4 24.8 37.2

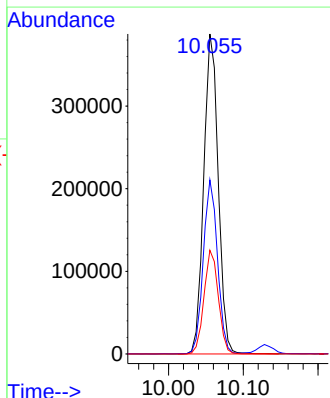



#64
Tetrachloroethene
Concen: 0.311 ug/l
RT: 9.275 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51




Instrument :
MSVOA_X
ClientSampleId :
DUP031622




Tgt Ion:164 Resp: 1260
Ion Ratio Lower Upper
164 100
166 120.7 101.2 151.8
129 104.0 73.0 109.4
131 69.5 74.2 111.2#

Manual Integrations
APPROVED



Reviewed By :John Carlone 03/24/2022
Supervised By :Mahesh Dadoda 03/24/2022

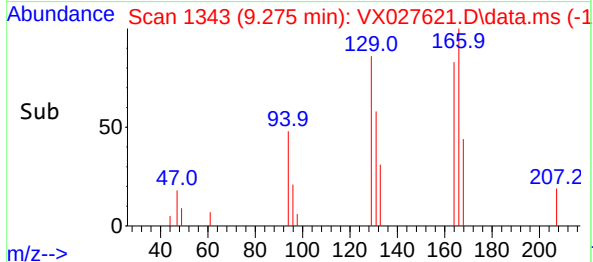


#67
Ethyl Benzene
Concen: 474.348 ug/l
RT: 10.201 min Scan# 1495
Delta R.T. 0.006 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51

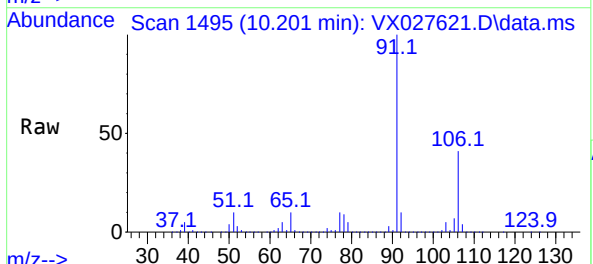

Tgt Ion: 91 Resp: 8699048
Ion Ratio Lower Upper
91 100
106 40.6 24.6 36.8#









#68
m/p-Xylenes
Concen: 1029.451 ug/l
RT: 10.311 min Scan# 1512
Delta R.T. 0.006 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51

Instrument :
MSVOA_X
ClientSampleId :
DUP031622

Tgt Ion:106 Resp: 743349
Ion Ratio Lower Upper
106 100
91 165.0 160.4 240.6




Manual Integrations
APPROVED


Reviewed By :John Carlone 03/24/2022
Supervised By :Mahesh Dadoda 03/24/2022

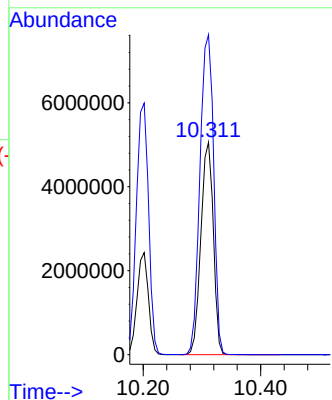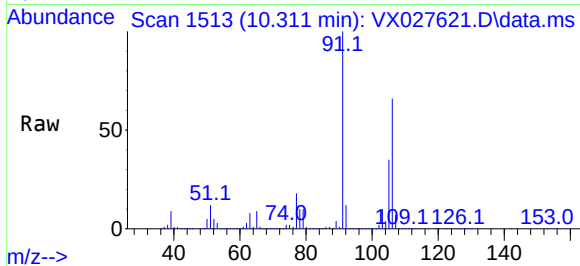

#69
o-Xylene
Concen: 323.985 ug/l
RT: 10.647 min Scan# 1568
Delta R.T. 0.000 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51


Tgt Ion:106 Resp: 2271469
Ion Ratio Lower Upper
106 100
91 200.8 106.1 318.1

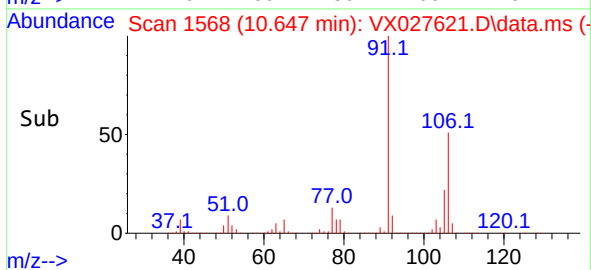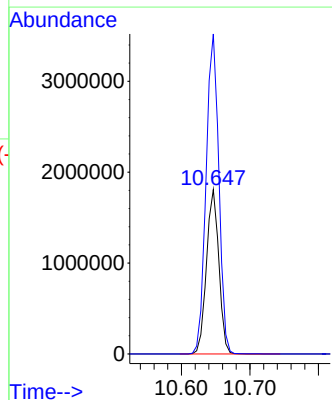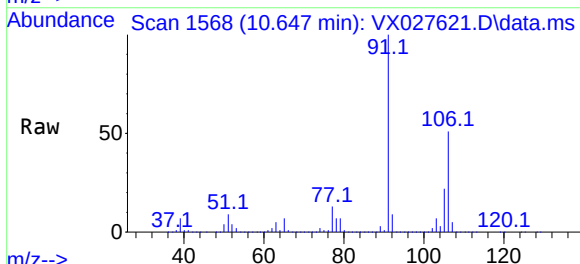



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51




Instrument :
MSVOA_X
ClientSampleId :
DUP031622




Tgt Ion:152 Resp: 24968
Ion Ratio Lower Upper
152 100
115 58.0 37.5 112.7
150 156.4 0.0 338.2

Manual Integrations
APPROVED



Reviewed By :John Carlone 03/24/2022
Supervised By :Mahesh Dadoda 03/24/2022

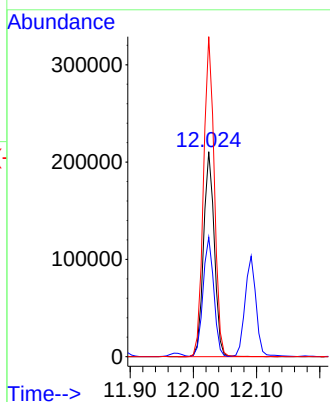


#73
Isopropylbenzene
Concen: 13.743 ug/l
RT: 10.964 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51




Tgt Ion:105 Resp: 249930
Ion Ratio Lower Upper
105 100
120 27.4 13.5 40.5





#78
n-propylbenzene
Concen: 53.994 ug/l
RT: 11.305 min Scan# 1077940
Delta R.T. 0.000 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51




Instrument :
MSVOA_X
ClientSampleId :
DUP031622




Tgt Ion: 91 Resp: 1077940
Ion Ratio Lower Upper
91 100
120 24.5 11.6 34.8

Manual Integrations
APPROVED



Reviewed By :John Carlone 03/24/2022
Supervised By :Mahesh Dadoda 03/24/2022




#80
1,3,5-Trimethylbenzene
Concen: 219.320 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.006 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51



Tgt Ion:105 Resp: 3357040
Ion Ratio Lower Upper
105 100
120 50.3 24.3 72.9

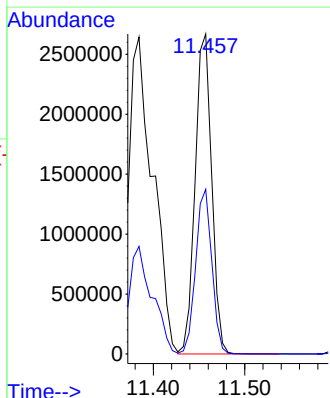



#83
tert-Butylbenzene
Concen: 11.730 ug/l
RT: 11.719 min Scan# 1744
Delta R.T. 0.000 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51

Instrument :

MSVOA_X

ClientSampleId :





DUP031622

Tgt Ion:119 Resp: 17786
Ion Ratio Lower Upper
119 100
91 65.5 26.9 80.6
134 24.2 11.4 34.2

Manual Integrations




APPROVED


Reviewed By :John Carlone 03/24/2022
Supervised By :Mahesh Dadoda 03/24/2022

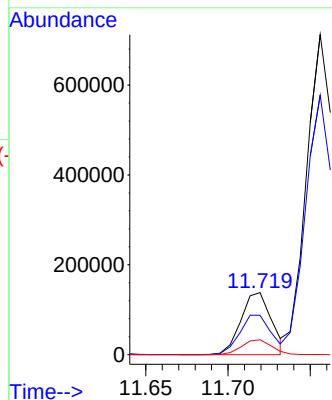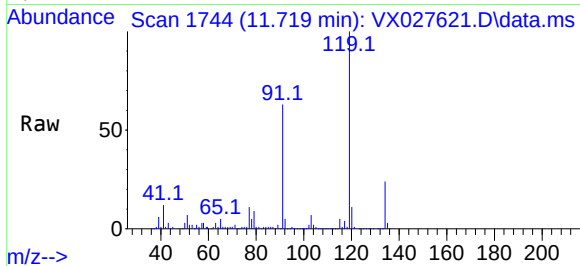

#84
1,2,4-Trimethylbenzene
Concen: 401.342 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.000 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51

Tgt Ion:105 Resp: 6126511
Ion Ratio Lower Upper
105 100
120 49.8 22.6 67.8

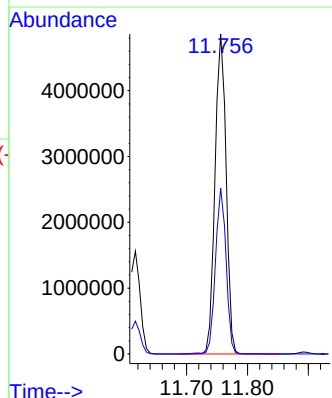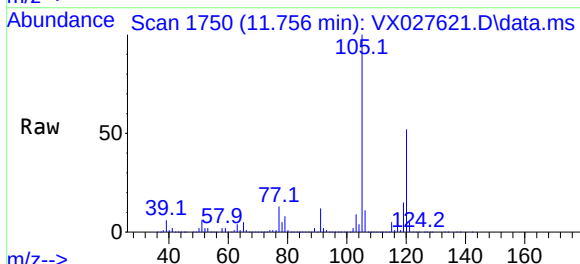







#85
 sec-Butylbenzene
 Concen: 2.040 ug/l m
 RT: 11.890 min Scan# 1772
 Delta R.T. 0.000 min
 Lab File: VX027621.D
 Acq: 22 Mar 2022 17:51

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP031622

Tgt Ion:105 Resp: 37378
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.2 30.4




Manual Integrations
 APPROVED


Reviewed By :John Carlone 03/24/2022
 Supervised By :Mahesh Dadoda 03/24/2022

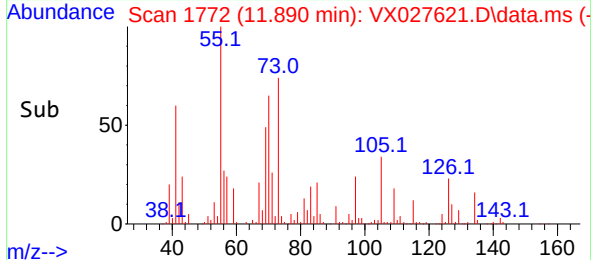

#86
 p-Isopropyltoluene
 Concen: 1.125 ug/l m
 RT: 12.012 min Scan# 1792
 Delta R.T. 0.000 min
 Lab File: VX027621.D
 Acq: 22 Mar 2022 17:51


Tgt Ion:119 Resp: 17704
 Ion Ratio Lower Upper
 119 100
 134 97.0 13.0 39.0#
 91 0.0 11.3 33.9#

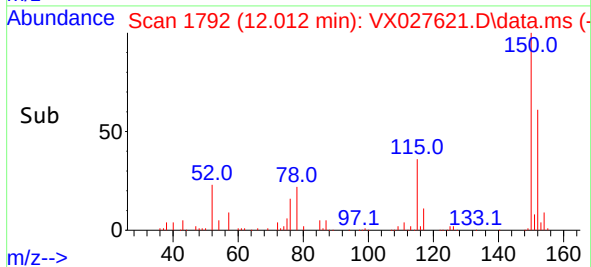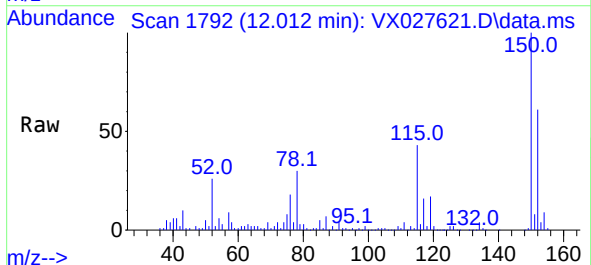



#91
1,2-Dichlorobenzene
Concen: 0.373 ug/l
RT: 12.341 min Scan# 1845
Delta R.T. 0.006 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51




Instrument :
MSVOA_X
ClientSampleId :
DUP031622

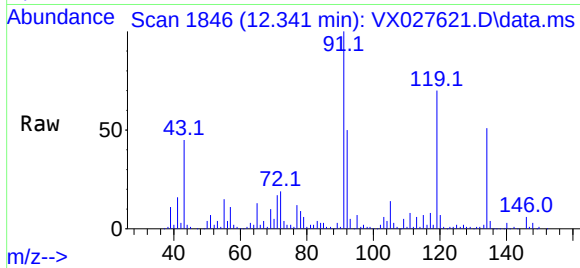


Tgt Ion:146 Resp: 309
Ion Ratio Lower Upper
146 100
111 100.6 21.0 63.0
148 69.3 32.6 97.7

Manual Integrations
APPROVED

Reviewed By :John Carlone 03/24/2022
Supervised By :Mahesh Dadoda 03/24/2022

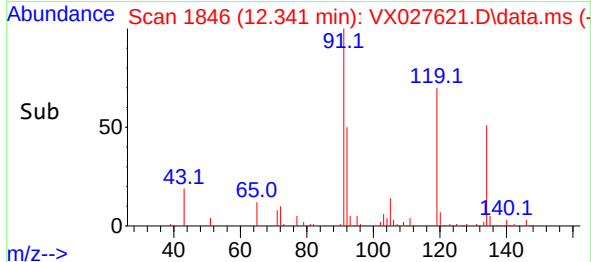

#95
Naphthalene
Concen: 132.830 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.000 min
Lab File: VX027621.D
Acq: 22 Mar 2022 17:51

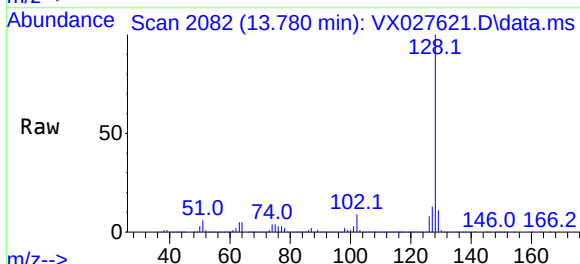

Tgt Ion:128 Resp: 2298478
Ion Ratio Lower Upper
128 100
127 13.1 10.2 15.4
129 11.4 8.7 13.1

