

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032222\
 Data File : VX027622.D
 Acq On : 22 Mar 2022 18:15
 Operator : JC/MD
 Sample : N1998-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M

Title : SW846 8260

Signal : TIC: VX027622.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	21	26	32	rBV	37253	66420	4.11%	0.758%
2	5.391	694	706	722	rBV	201996	583056	36.10%	6.652%
3	5.556	722	733	750	rVV	339364	960160	59.44%	10.955%
4	5.964	789	800	820	rBV	195672	525634	32.54%	5.997%
5	6.763	921	931	946	rBV	509458	1214061	75.16%	13.852%
6	8.653	1234	1241	1249	rBV	1052184	1615221	100.00%	18.428%
7	10.055	1465	1471	1485	rBV	1034113	1387739	85.92%	15.833%
8	10.195	1490	1494	1502	rVV	23284	32148	1.99%	0.367%
9	10.305	1506	1512	1523	rBV	45529	64658	4.00%	0.738%
10	11.085	1634	1640	1651	rBV	784341	1025032	63.46%	11.695%
11	11.756	1745	1750	1755	rVB	23535	28526	1.77%	0.325%
12	12.024	1789	1794	1801	rBV	1063662	1262147	78.14%	14.400%




Sum of corrected areas: 8764802

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032222\
Data File : VX027622.D
Acq On : 22 Mar 2022 18:15
Operator : JC/MD
Sample : N1998-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

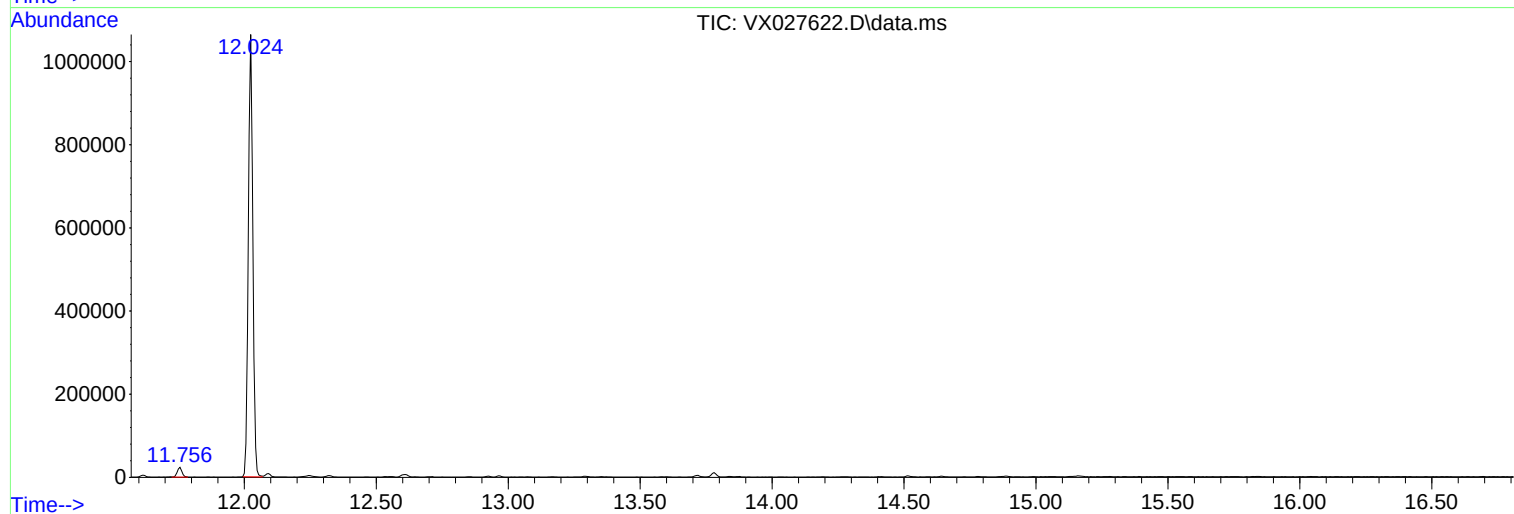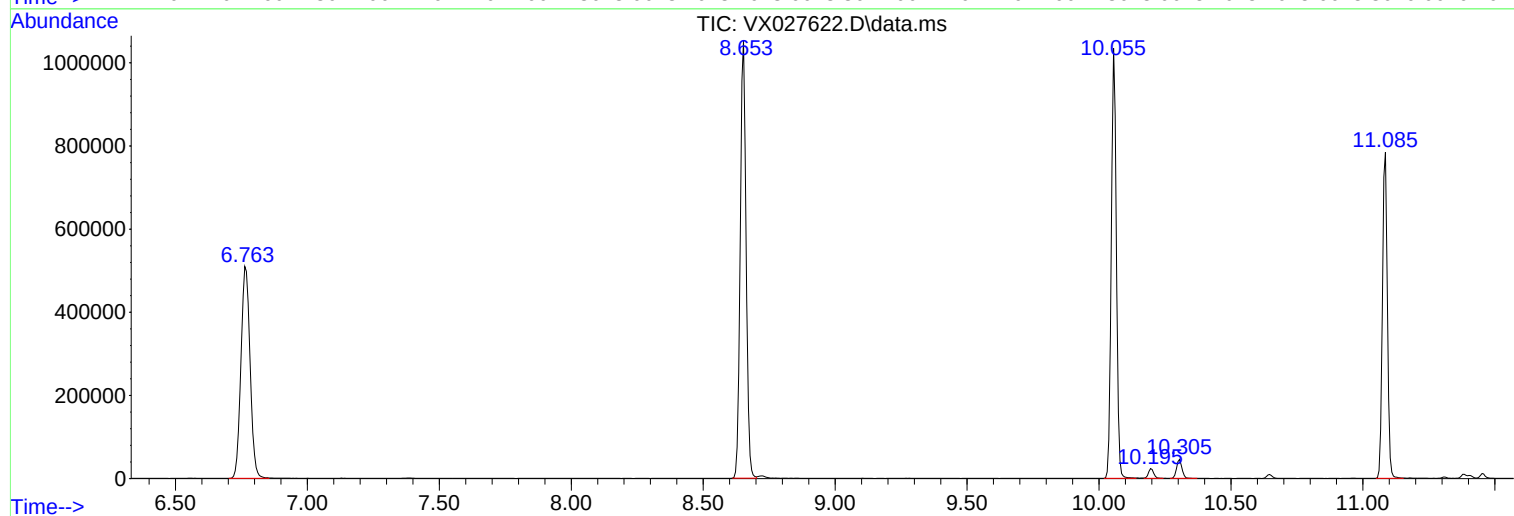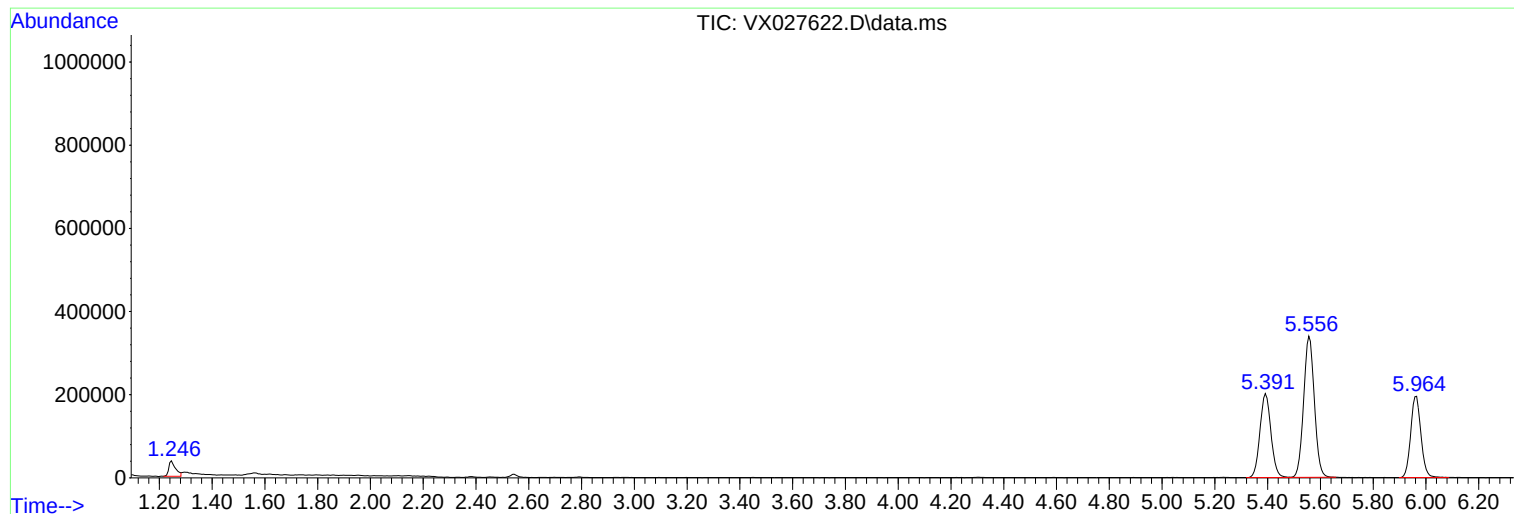

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032222\
Data File : VX027622.D
Acq On : 22 Mar 2022 18:15
Operator : JC/MD
Sample : N1998-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032222\
Data File : VX027622.D
Acq On : 22 Mar 2022 18:15
Operator : JC/MD
Sample : N1998-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------