

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032222\
 Data File : VX027627.D
 Acq On : 22 Mar 2022 20:13
 Operator : JC/MD
 Sample : N2028-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-118

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
 Title : SW846 8260

Signal : TIC: VX027627.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	20	29	43	rBV	178509	624004	37.98%	6.519%
2	1.745	105	108	130	rVB3	23128	85117	5.18%	0.889%
3	2.386	208	213	221	rVB	12816	20937	1.27%	0.219%
4	5.391	693	706	721	rBV2	195870	567480	34.54%	5.929%
5	5.556	721	733	753	rVB	344872	971662	59.13%	10.151%
6	5.958	788	799	810	rBV	200223	523532	31.86%	5.469%
7	6.245	836	846	856	rBV5	8337	23850	1.45%	0.249%
8	6.763	921	931	945	rBV	504832	1215984	74.00%	12.704%
9	8.427	1198	1204	1213	rBV	15105	27094	1.65%	0.283%
10	8.653	1234	1241	1248	rVV	1046838	1643179	100.00%	17.167%
11	8.720	1248	1252	1260	rVB	14196	25268	1.54%	0.264%
12	9.457	1366	1373	1381	rBV2	28492	48305	2.94%	0.505%
13	10.055	1466	1471	1483	rVB	1025388	1357098	82.59%	14.178%
14	10.305	1506	1512	1518	rBV	23213	33175	2.02%	0.347%
15	11.085	1634	1640	1649	rBV	849861	1088442	66.24%	11.371%
16	12.024	1788	1794	1802	rBV	1072675	1316808	80.14%	13.757%




Sum of corrected areas: 9571935

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032222\
Data File : VX027627.D
Acq On : 22 Mar 2022 20:13
Operator : JC/MD
Sample : N2028-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-118

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

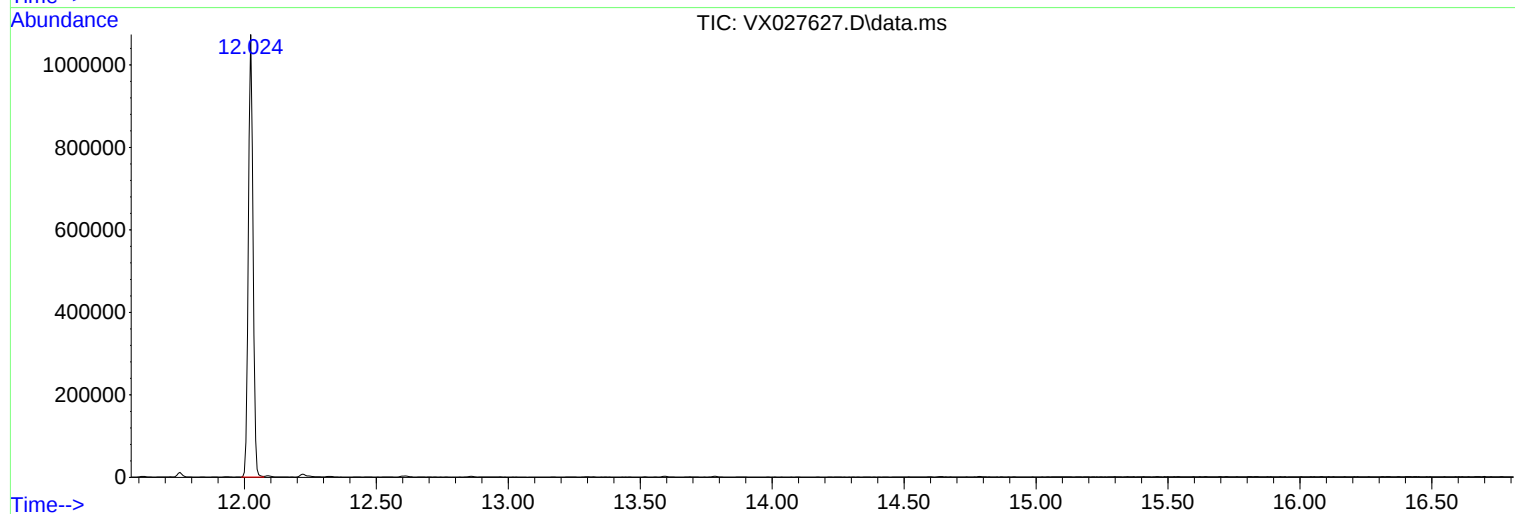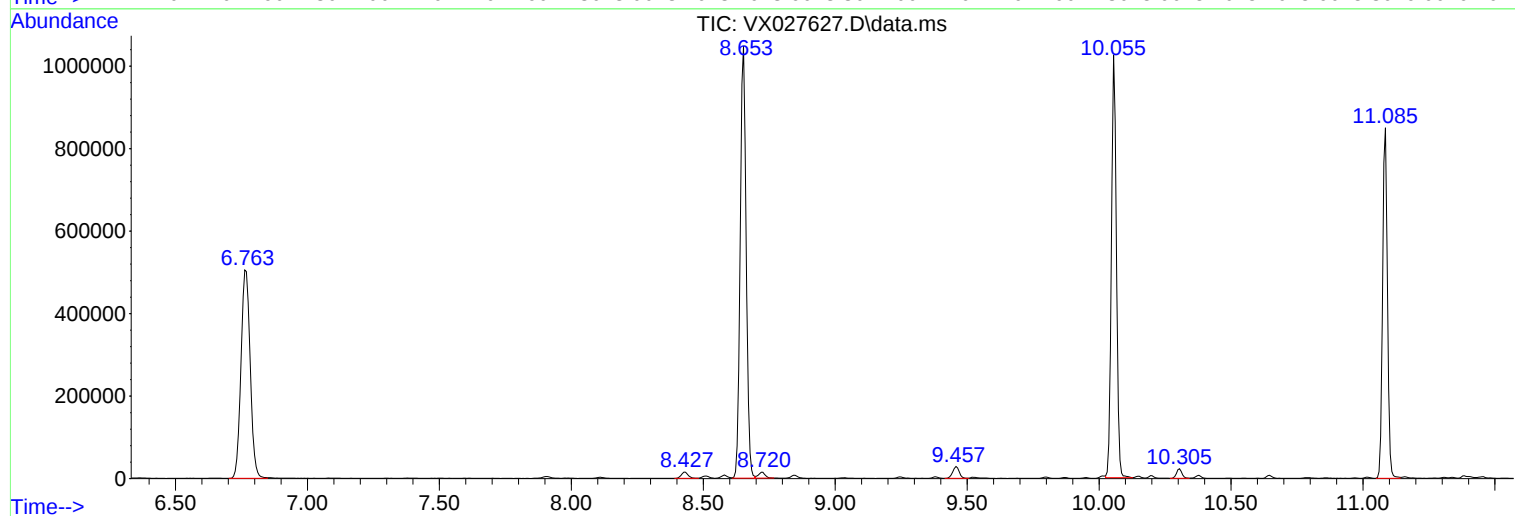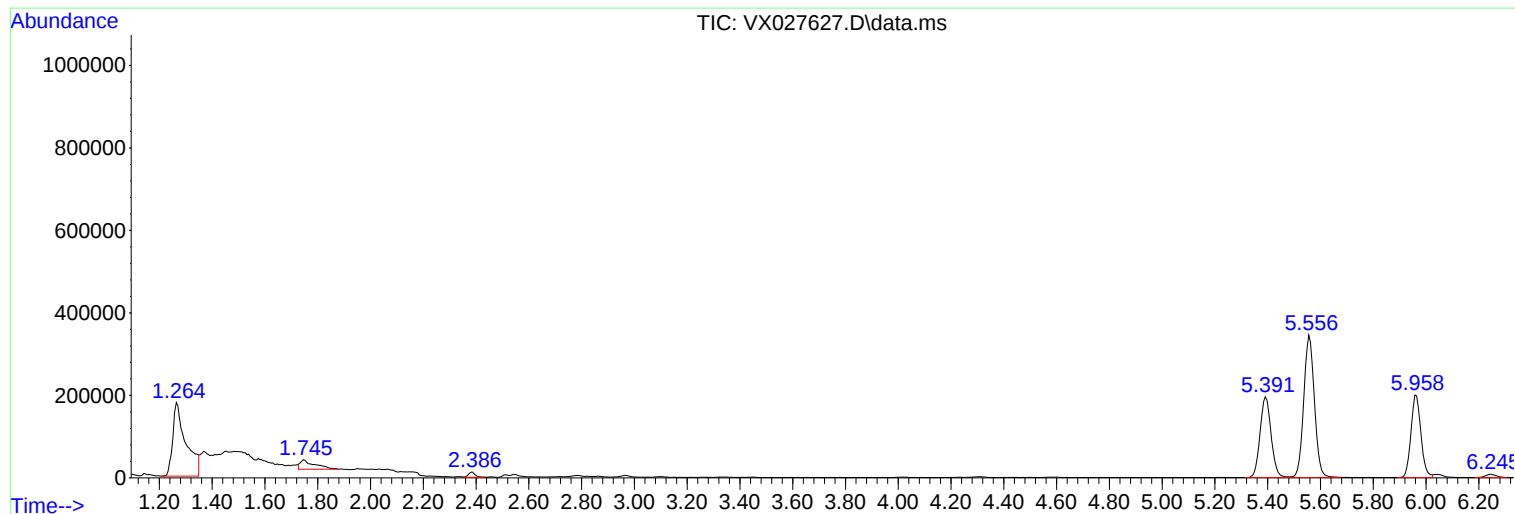

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032222\
Data File : VX027627.D
Acq On : 22 Mar 2022 20:13
Operator : JC/MD
Sample : N2028-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-118








Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.264	32.11 ug/l	624004	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	90
2			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	64
3			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
4			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	5
5			Ethene, 1,2-difluoro-	64	C2H2F2	001691-13-0	4

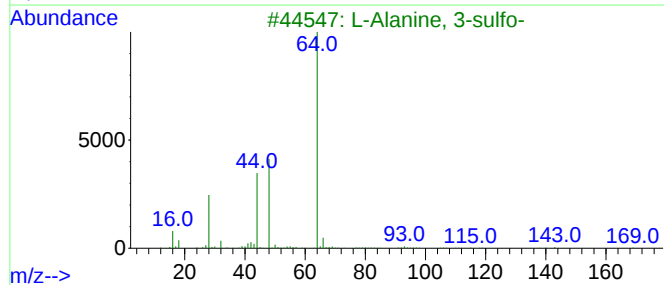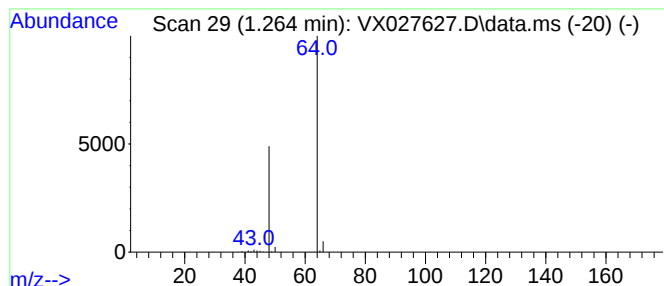

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032222\
Data File : VX027627.D
Acq On : 22 Mar 2022 20:13
Operator : JC/MD
Sample : N2028-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-118

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.264	32.1	ug/l	624004	1	5.556	971662	50.0