

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032222\
 Data File : VX027638.D
 Acq On : 23 Mar 2022 01:46
 Operator : JC/MD
 Sample : N2062-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-3

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
 Title : SW846 8260

Signal : TIC: VX027638.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	21	26	32	rBV	28487	52732	3.37%	0.516%
2	2.538	229	238	248	rBV	15901	28425	1.82%	0.278%
3	5.391	694	706	721	rBV	197379	568495	36.33%	5.560%
4	5.556	721	733	750	rVB	333252	943000	60.27%	9.222%
5	5.958	788	799	822	rBV	190076	502487	32.11%	4.914%
6	6.763	920	931	946	rBV	461440	1121116	71.65%	10.964%
7	8.653	1234	1241	1256	rVB	980916	1564748	100.00%	15.302%
8	10.055	1465	1471	1479	rBV	1041888	1390815	88.88%	13.601%
9	11.085	1634	1640	1646	rBV	838732	1081319	69.10%	10.575%
10	11.890	1769	1772	1779	rVB	16681	22119	1.41%	0.216%
11	12.024	1789	1794	1809	rVB	1083266	1314512	84.01%	12.855%
12	12.177	1815	1819	1824	rBV	38874	50124	3.20%	0.490%
13	12.250	1824	1831	1835	rVV	48935	70326	4.49%	0.688%
14	12.317	1835	1842	1855	rVB3	26366	47716	3.05%	0.467%
15	12.646	1892	1896	1902	rBV	22627	37086	2.37%	0.363%
16	12.701	1902	1905	1911	rVV	17925	26353	1.68%	0.258%
17	12.762	1911	1915	1920	rVB	15591	19697	1.26%	0.193%
18	12.841	1921	1928	1933	rBV	56396	77844	4.97%	0.761%
19	12.902	1933	1938	1945	rVB3	13975	27159	1.74%	0.266%
20	13.036	1955	1960	1964	rBV	38756	49923	3.19%	0.488%
21	13.140	1968	1977	1979	rBV2	24557	44498	2.84%	0.435%
22	13.195	1979	1986	1992	rVB3	58419	114781	7.34%	1.122%
23	13.353	2007	2012	2015	rBV2	19185	27797	1.78%	0.272%
24	13.621	2052	2056	2057	rVV	49030	57443	3.67%	0.562%
25	13.664	2057	2063	2074	rVB	267659	424824	27.15%	4.155%
26	13.756	2074	2078	2081	rBV	18763	25566	1.63%	0.250%
27	13.798	2081	2085	2090	rVB2	14137	27915	1.78%	0.273%
28	13.853	2090	2094	2099	rBV2	13363	18804	1.20%	0.184%
29	13.926	2101	2106	2110	rVB	72549	87538	5.59%	0.856%
30	13.975	2110	2114	2117	rBV2	16401	19513	1.25%	0.191%
31	14.103	2131	2135	2142	rVB6	13484	24664	1.58%	0.241%
32	14.268	2155	2162	2163	rVV2	8630	19758	1.26%	0.193%
33	14.286	2163	2165	2168	rVV2	18406	19514	1.25%	0.191%
34	14.377	2175	2180	2185	rVB	27159	39946	2.55%	0.391%
35	14.487	2192	2198	2202	rBV2	26335	43585	2.79%	0.426%
36	14.640	2217	2223	2226	rBV3	16498	24695	1.58%	0.242%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032222\
Data File : VX027638.D
Acq On : 23 Mar 2022 01:46
Operator : JC/MD
Sample : N2062-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M

Title : SW846 8260

37	14.676	2226	2229	2233	rVB	25625	32812	2.10%	0.321%
38	14.792	2241	2248	2251	rBV	32409	49285	3.15%	0.482%
39	14.920	2261	2269	2277	rBV3	20846	53291	3.41%	0.521%
40	15.176	2305	2311	2320	rBV2	16220	31978	2.04%	0.313%
41	15.261	2320	2325	2330	rVV2	16774	24396	1.56%	0.239%
42	15.597	2374	2380	2386	rVB4	9127	16929	1.08%	0.166%


Sum of corrected areas: 10225528

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032222\
Data File : VX027638.D
Acq On : 23 Mar 2022 01:46
Operator : JC/MD
Sample : N2062-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

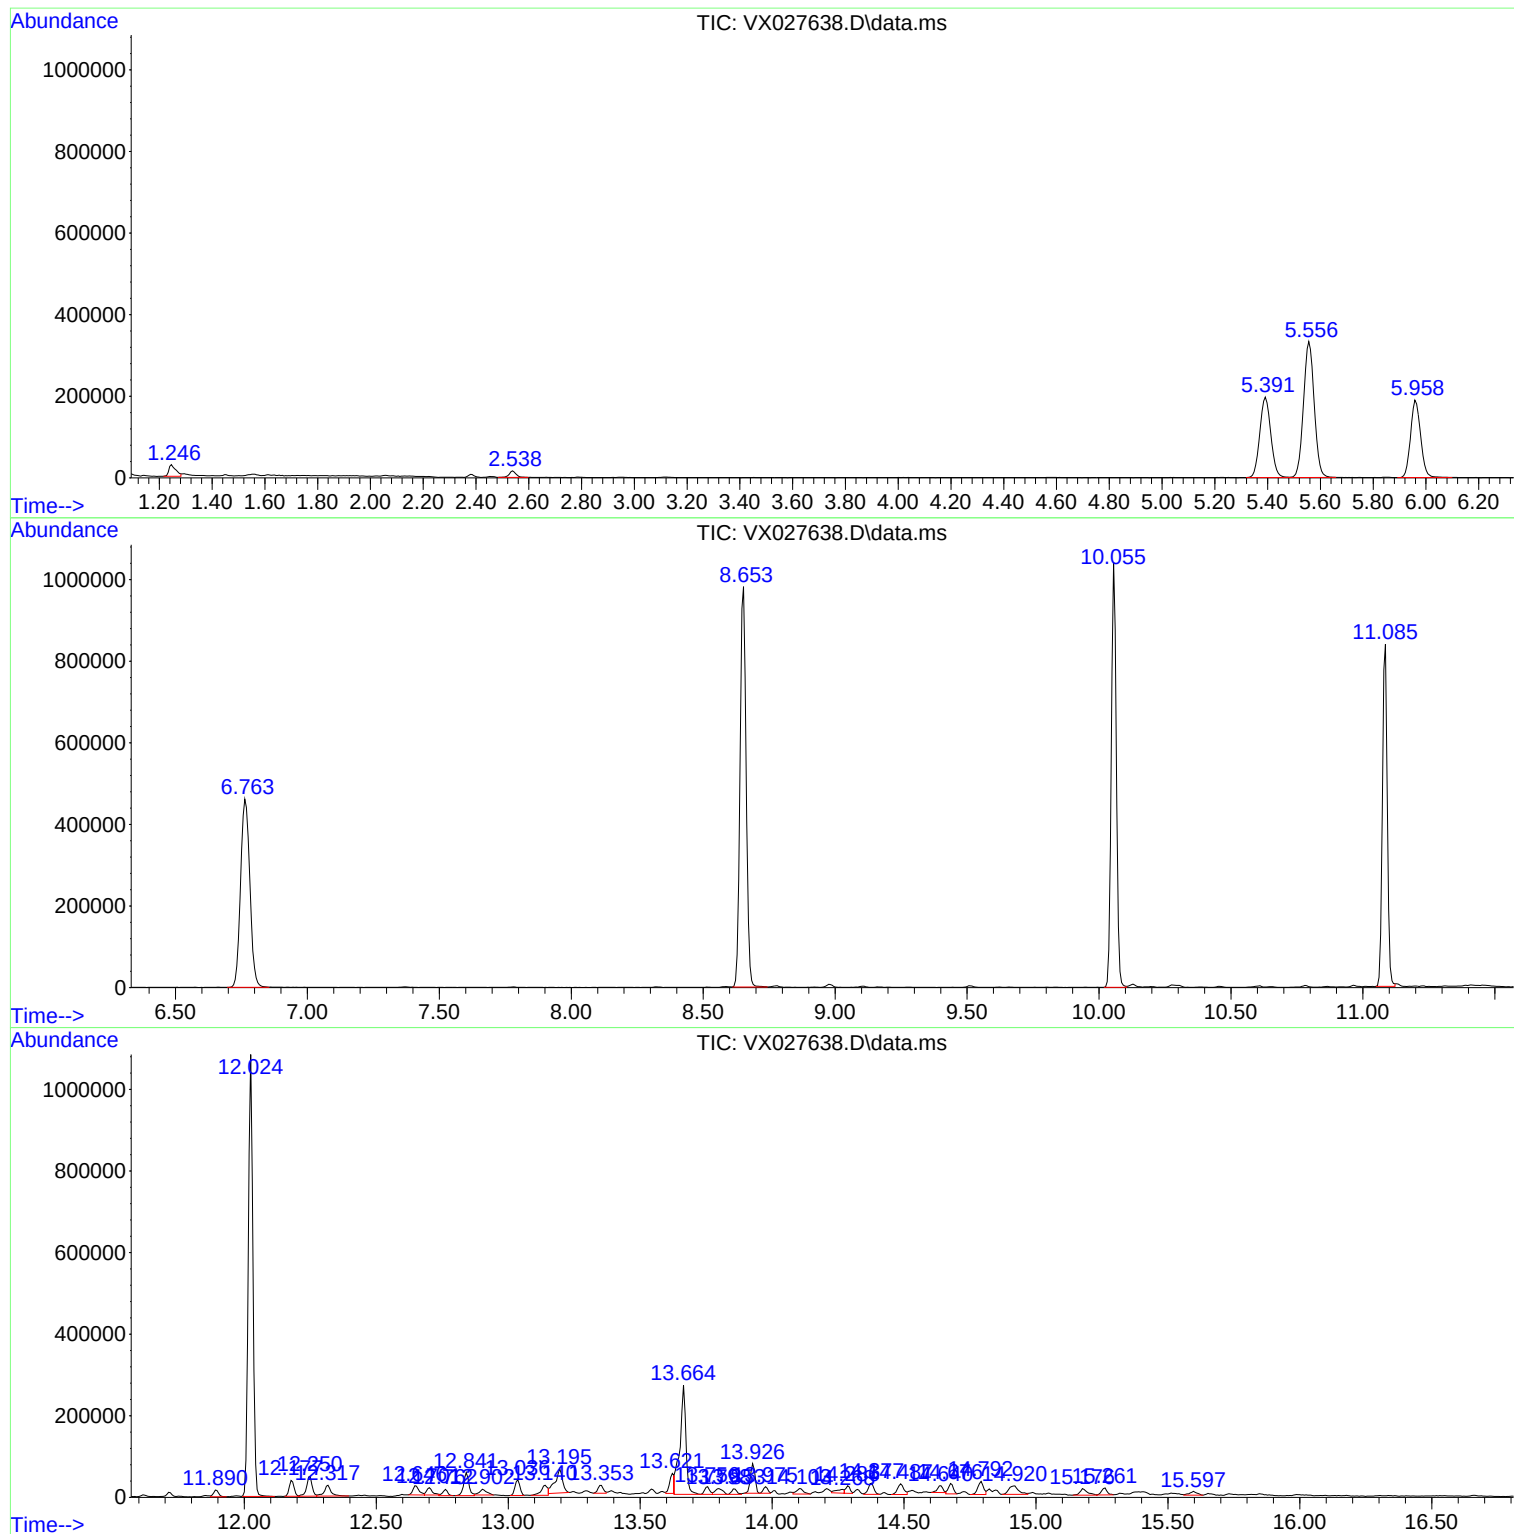

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032222\
Data File : VX027638.D
Acq On : 23 Mar 2022 01:46
Operator : JC/MD
Sample : N2062-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1H-Indene, 2,3-dihydro-1,3-... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.664	16.16 ug/l	424824	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1H-Indene, 2,3-dihydro-1,3-dimet...	146	C11H14	004175-53-5	94
2			Naphthalene, 1,2,3,4-tetrahydro-...	146	C11H14	001559-81-5	91
3			1H-Indene, 2,3-dihydro-4,7-dimet...	146	C11H14	006682-71-9	91
4			Benzene, (3-methyl-2-butenyl)-	146	C11H14	004489-84-3	91
5			1H-Indene, 2,3-dihydro-1,6-dimet...	146	C11H14	017059-48-2	91

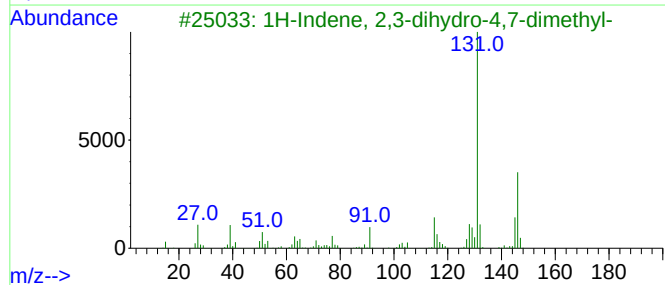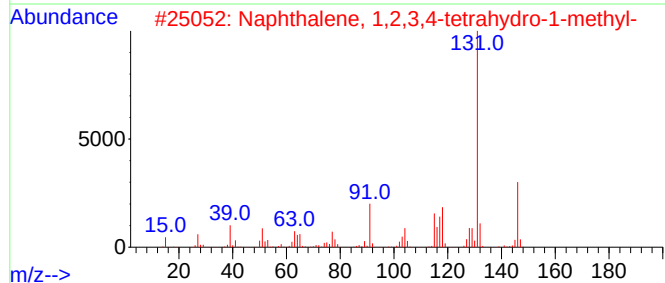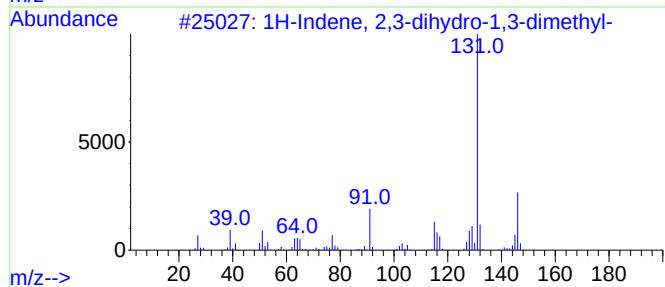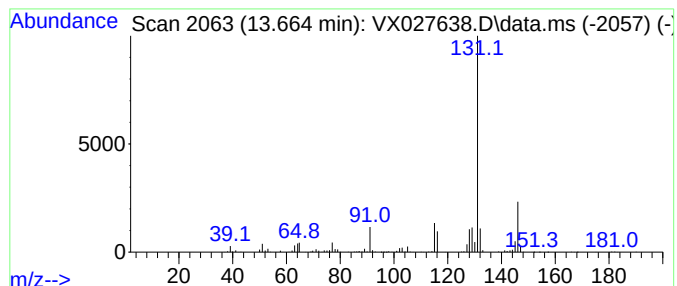

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032222\
Data File : VX027638.D
Acq On : 23 Mar 2022 01:46
Operator : JC/MD
Sample : N2062-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1H-Indene, 2,3-...	13.664	16.2	ug/l	424824	4	12.024	1314510	50.0