

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032222\
 Data File : VX027641.D
 Acq On : 23 Mar 2022 02:56
 Operator : JC/MD
 Sample : N2062-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-6

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
 Title : SW846 8260

Signal : TIC: VX027641.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	42	rBV	28491	64976	4.15%	0.688%
2	2.538	230	238	249	rBV	11855	21699	1.39%	0.230%
3	3.117	325	333	343	rBV2	25055	59053	3.77%	0.625%
4	5.391	691	706	722	rBV	206400	603448	38.54%	6.391%
5	5.556	722	733	750	rVB	352533	998783	63.78%	10.578%
6	5.958	789	799	814	rBV	203236	537748	34.34%	5.695%
7	6.763	920	931	945	rBV	536688	1275095	81.43%	13.504%
8	8.653	1233	1241	1257	rBV	995336	1565913	100.00%	16.584%
9	10.055	1465	1471	1480	rBV	1113444	1491001	95.22%	15.791%
10	11.085	1634	1640	1653	rBV	852940	1131149	72.24%	11.980%
11	11.890	1769	1772	1777	rVB	14204	18685	1.19%	0.198%
12	12.024	1788	1794	1806	rBV	1111762	1360972	86.91%	14.414%
13	12.250	1823	1831	1836	rBV2	18737	28826	1.84%	0.305%
14	12.317	1836	1842	1851	rVB3	11929	22055	1.41%	0.234%
15	12.646	1892	1896	1902	rBV2	19544	29456	1.88%	0.312%
16	12.841	1924	1928	1934	rVB	16129	20899	1.33%	0.221%
17	13.140	1969	1977	1979	rBV	12614	17735	1.13%	0.188%
18	13.195	1979	1986	1992	rVB3	13535	27413	1.75%	0.290%
19	13.640	2052	2059	2061	rBV2	20156	42633	2.72%	0.452%
20	13.664	2061	2063	2074	rVB2	30681	45400	2.90%	0.481%
21	13.926	2099	2106	2110	rVB	24383	32380	2.07%	0.343%
22	14.378	2174	2180	2185	rVB4	11569	18844	1.20%	0.200%
23	14.792	2240	2248	2256	rBV	14080	28143	1.80%	0.298%




Sum of corrected areas: 9442306

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032222\
Data File : VX027641.D
Acq On : 23 Mar 2022 02:56
Operator : JC/MD
Sample : N2062-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

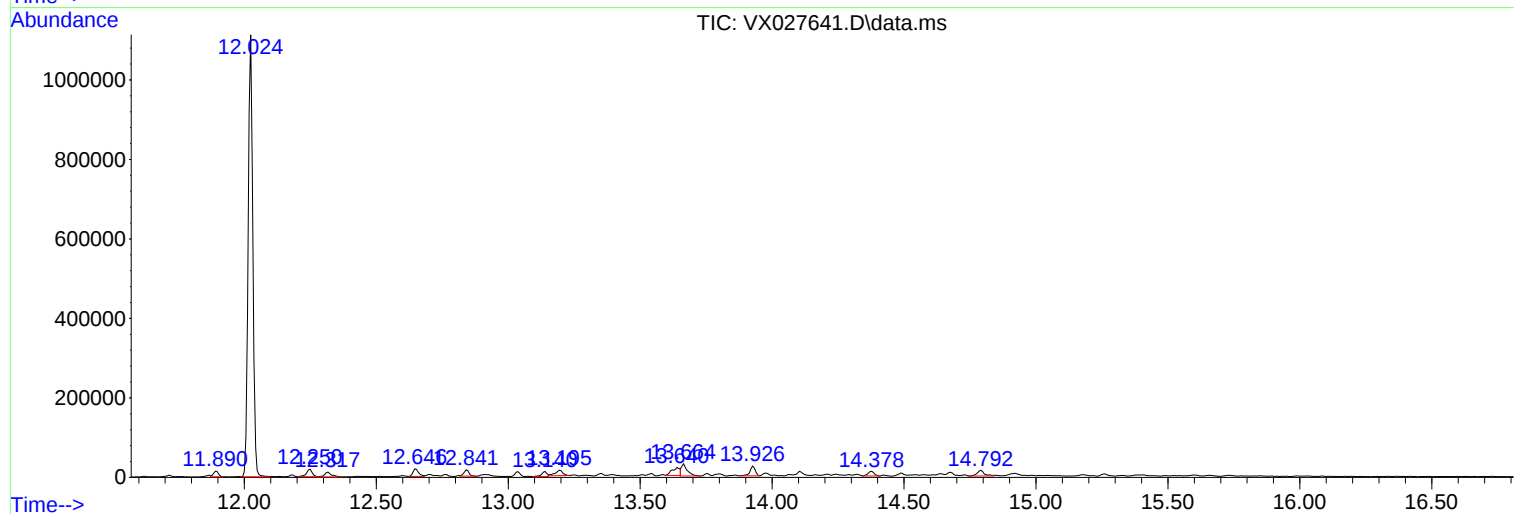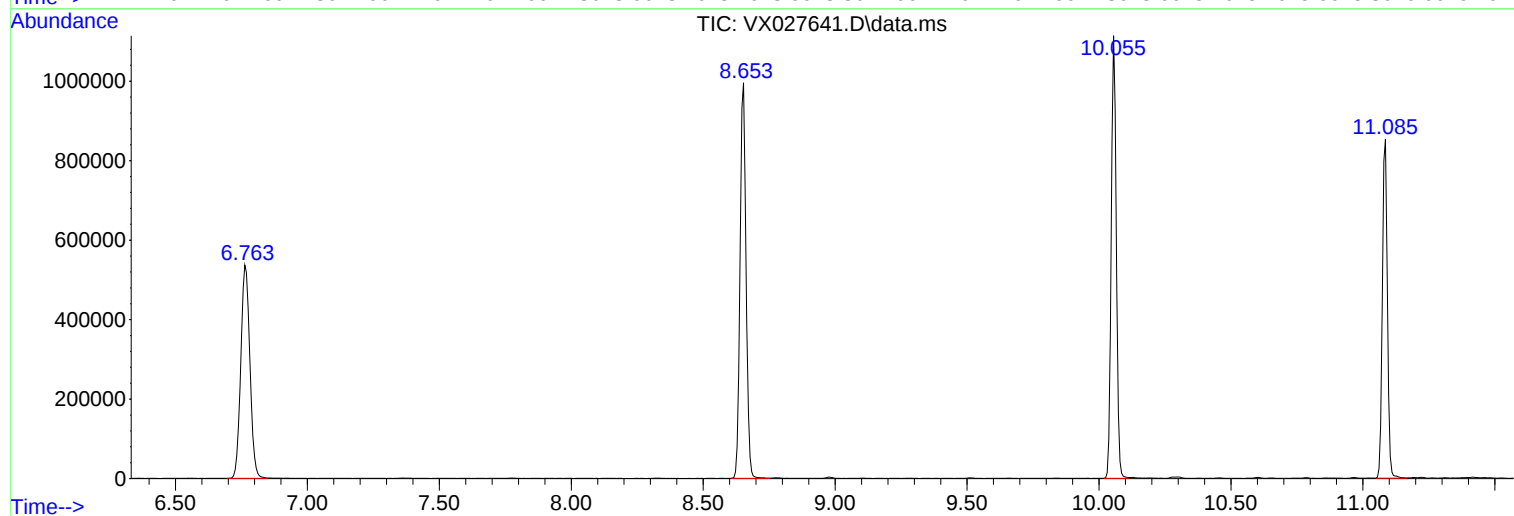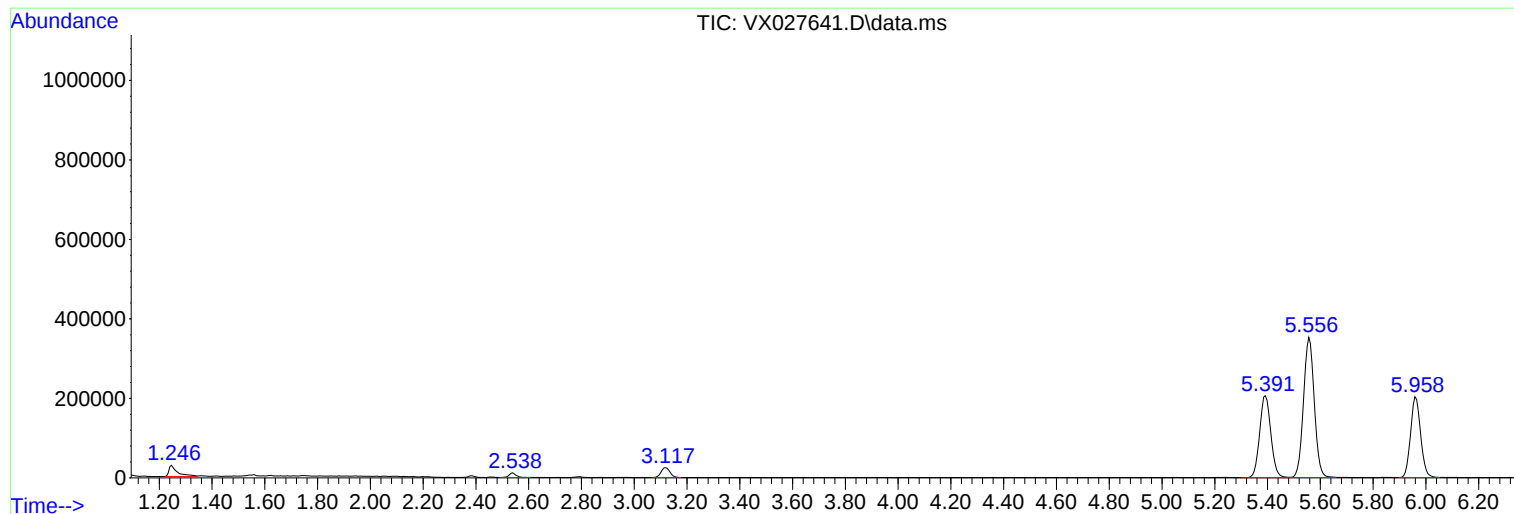

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032222\
Data File : VX027641.D
Acq On : 23 Mar 2022 02:56
Operator : JC/MD
Sample : N2062-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032222\
Data File : VX027641.D
Acq On : 23 Mar 2022 02:56
Operator : JC/MD
Sample : N2062-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------