

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032222\
 Data File : VX027645.D
 Acq On : 23 Mar 2022 04:30
 Operator : JC/MD
 Sample : N2028-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-123

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
 Title : SW846 8260

Signal : TIC: VX027645.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	21	26	40	rBV2	24518	60847	3.62%	0.587%
2	3.117	323	333	351	rBV	583563	1329514	79.13%	12.835%
3	5.391	694	706	722	rBV	208236	602530	35.86%	5.817%
4	5.556	722	733	747	rVB	348063	990892	58.98%	9.566%
5	5.958	789	799	817	rBV	203656	542106	32.27%	5.234%
6	6.763	921	931	945	rBV	528306	1251621	74.50%	12.083%
7	8.653	1233	1241	1258	rBV	1068465	1680096	100.00%	16.220%
8	9.244	1332	1338	1352	rVB	26280	42058	2.50%	0.406%
9	9.458	1366	1373	1380	rBV	17773	26057	1.55%	0.252%
10	10.055	1465	1471	1484	rBV	1085246	1448617	86.22%	13.985%
11	11.085	1634	1640	1652	rBV	833826	1088686	64.80%	10.510%
12	12.024	1789	1794	1802	rBV	1083517	1295246	77.09%	12.504%




Sum of corrected areas: 10358270

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032222\
Data File : VX027645.D
Acq On : 23 Mar 2022 04:30
Operator : JC/MD
Sample : N2028-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-123

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

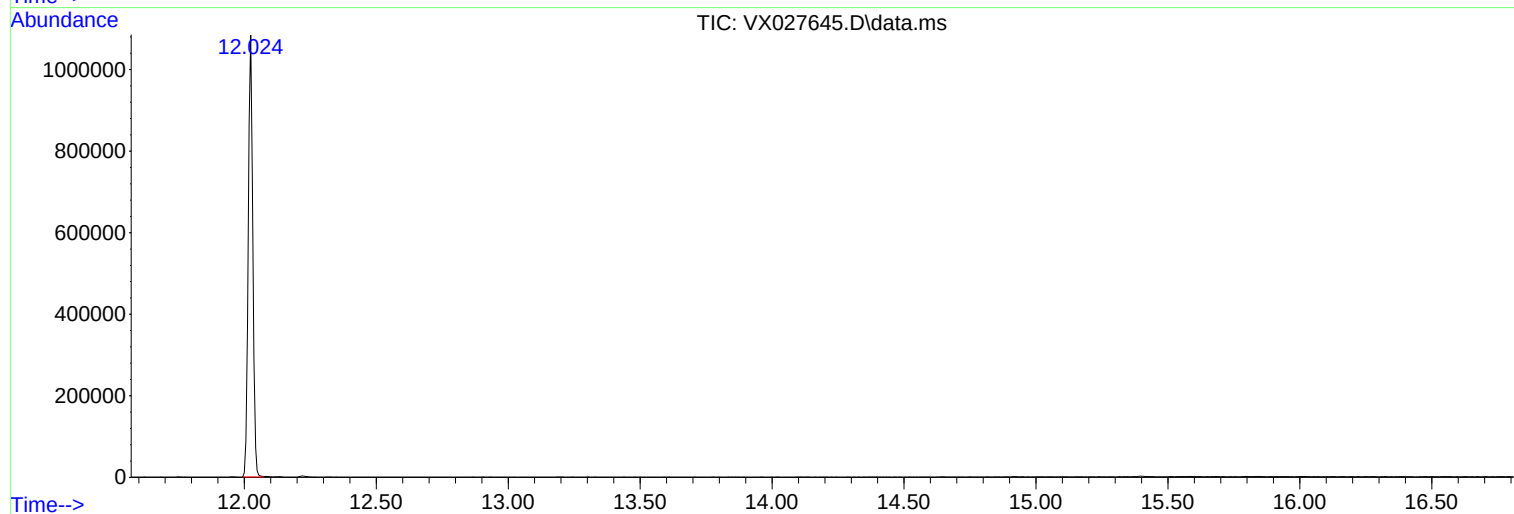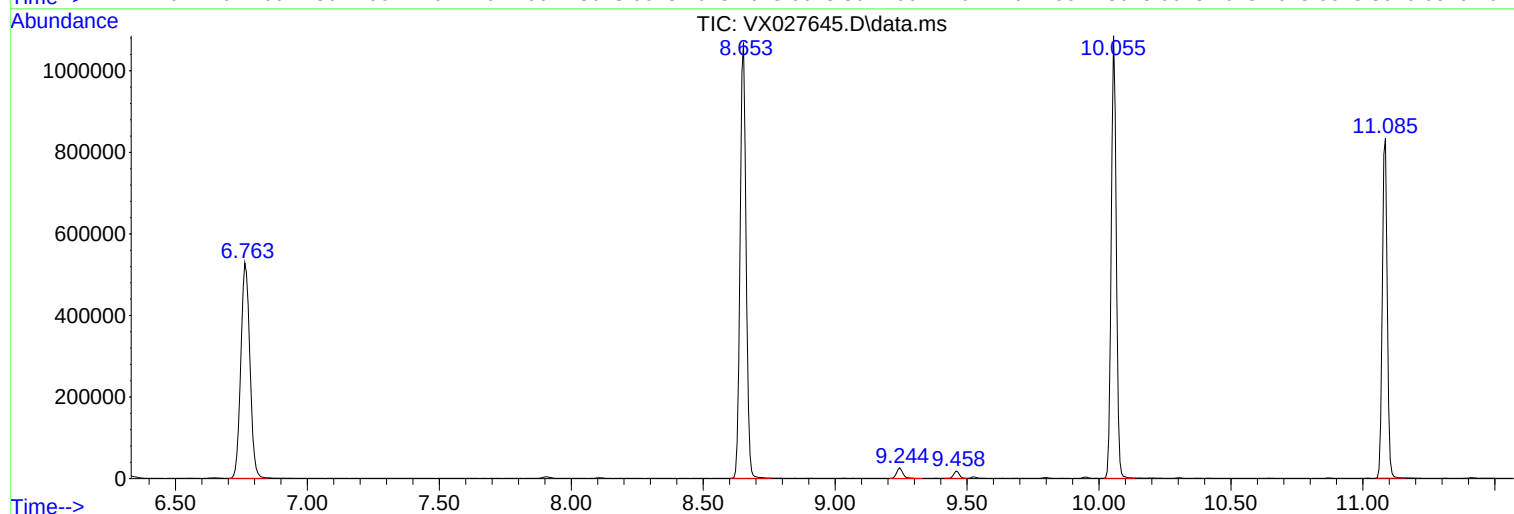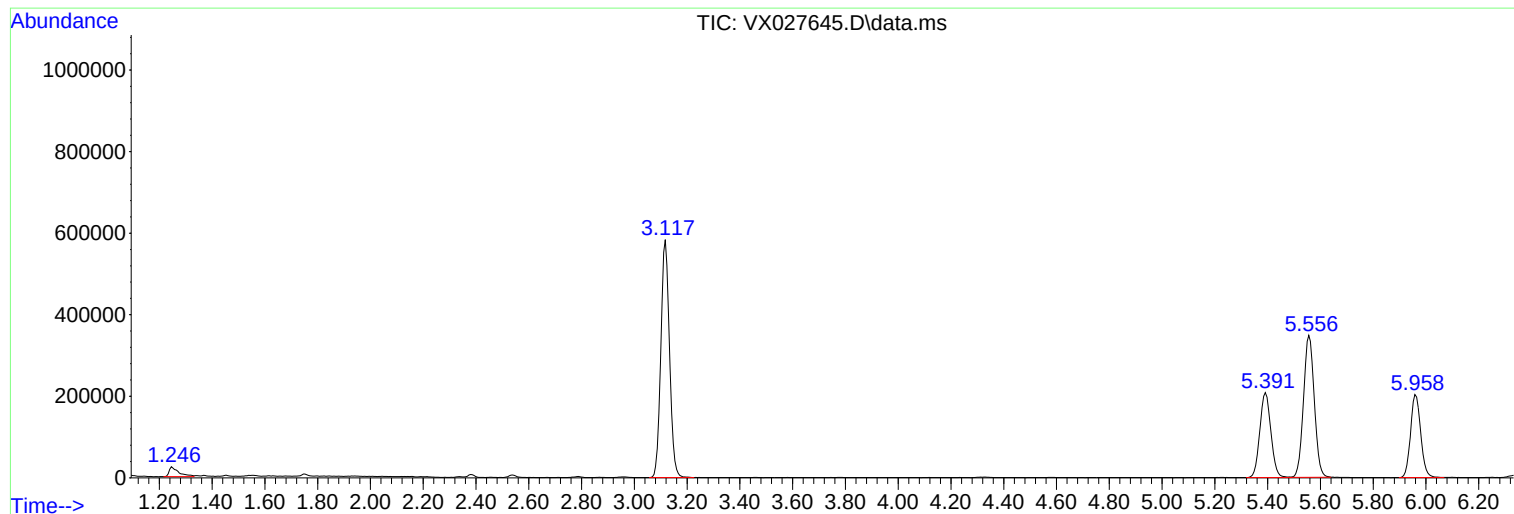

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032222\
Data File : VX027645.D
Acq On : 23 Mar 2022 04:30
Operator : JC/MD
Sample : N2028-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-123

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032222\
Data File : VX027645.D
Acq On : 23 Mar 2022 04:30
Operator : JC/MD
Sample : N2028-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-123

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------