
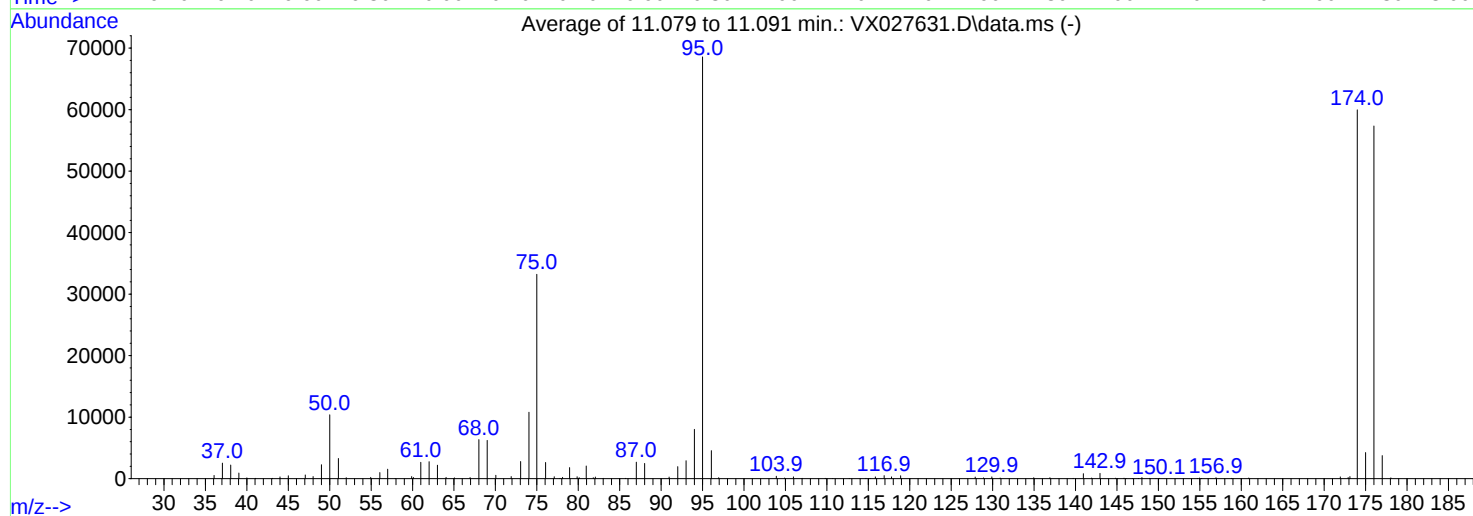


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032222\
 Data File : VX027631.D
 Acq On : 22 Mar 2022 22:11
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
 Title : SW846 8260
 Last Update : Thu Mar 17 15:02:59 2022

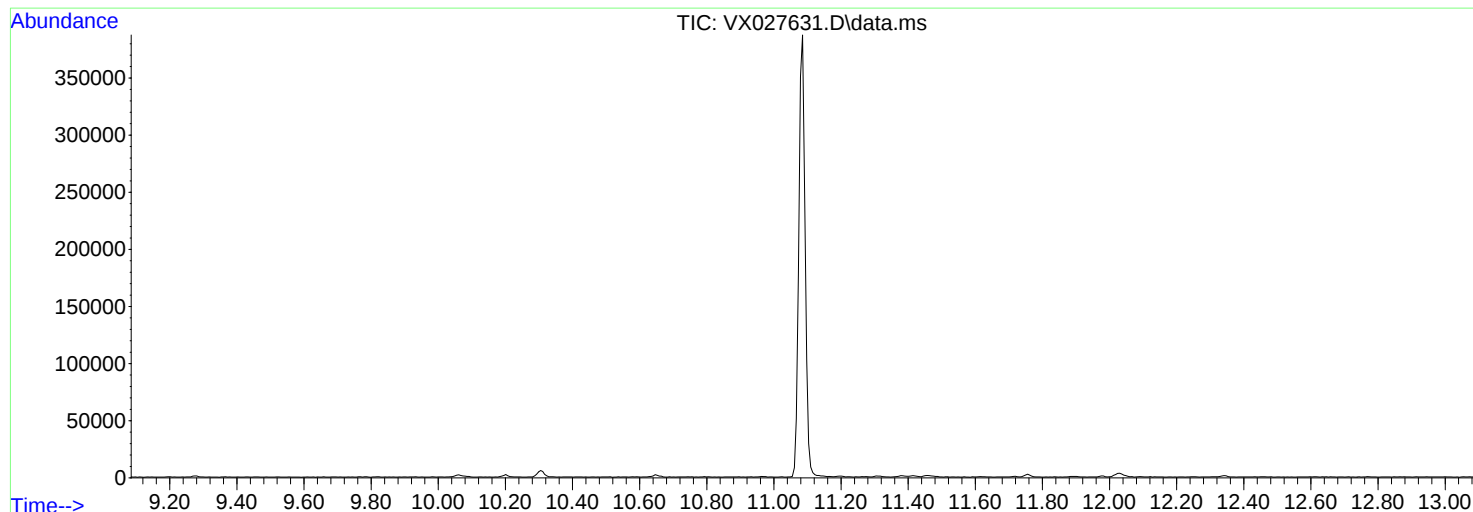

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.1	10379	PASS
75	95	30	60	48.4	33227	PASS
95	95	100	100	100.0	68581	PASS
96	95	5	9	6.6	4557	PASS
173	174	0.00	2	0.6	355	PASS
174	95	50	100	87.4	59957	PASS
175	174	5	9	7.1	4255	PASS
176	174	95	101	95.6	57341	PASS
177	176	5	9	6.5	3743	PASS