



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032223\
Data File : VX034660.D
Acq On : 22 Mar 2023 08:28
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Title : SW846 8260
Last Update : Mon Mar 13 10:29:32 2023

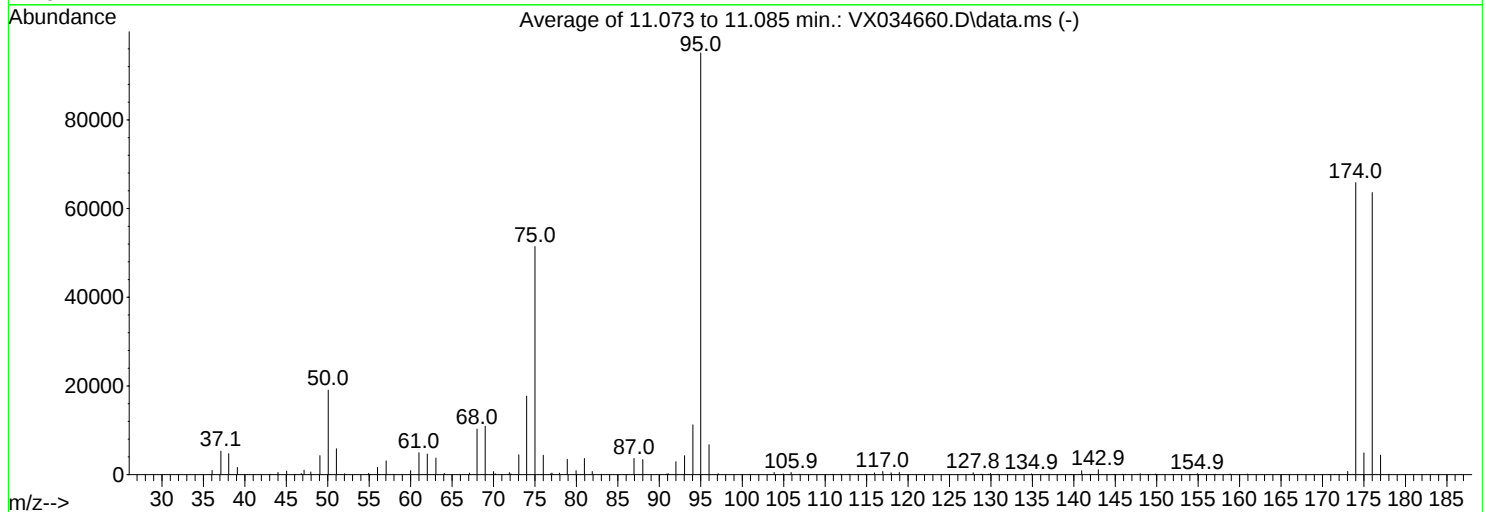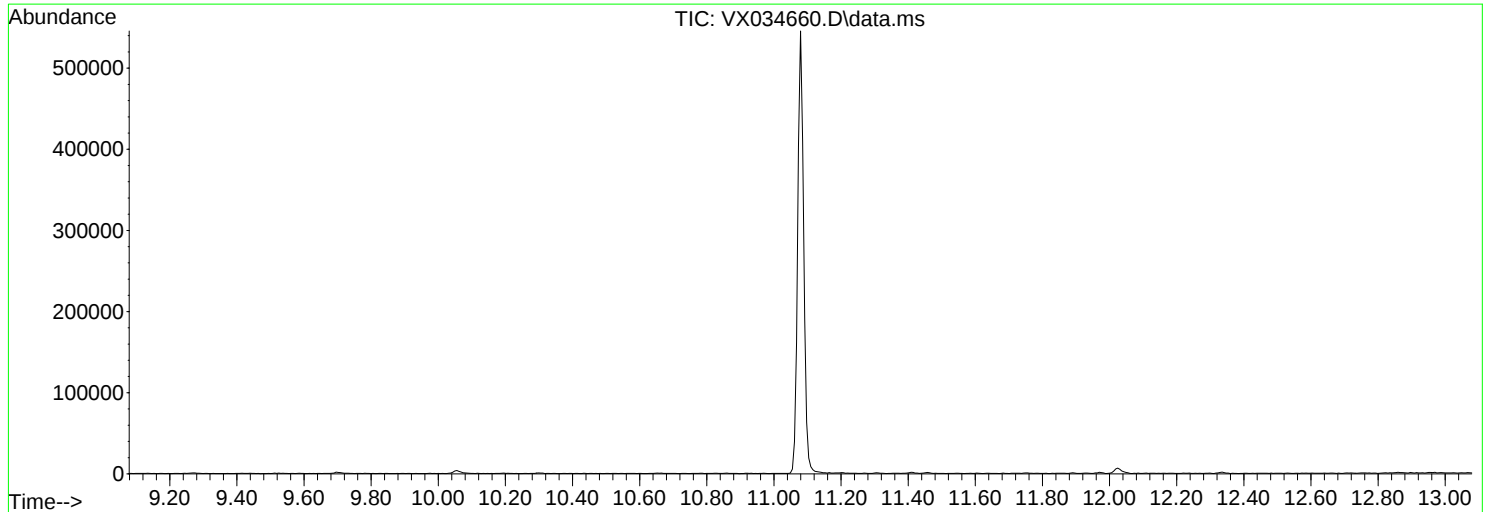

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.0	19049	PASS
75	95	30	60	54.1	51451	PASS
95	95	100	100	100.0	95115	PASS
96	95	5	9	7.1	6765	PASS
173	174	0.00	2	1.1	711	PASS
174	95	50	100	69.2	65848	PASS
175	174	5	9	7.5	4927	PASS
176	174	95	101	96.6	63597	PASS
177	176	5	9	6.9	4412	PASS