

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX032319\  
Data File : VX008365.D  
Acq On : 23 Mar 2019 21:16  
Operator : JC/SP  
Sample : K1937-15  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BPS1-TT-MW307S-20190314

## Integration Parameters: RTEINT.P

Integrator: RTE  
Smoothing : ON Filtering: 5  
Sampling : 1 Min Area: 3 % of largest Peak  
Start Thrs: 0.2 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X032319W.M  
Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.617       | 64            | 76          | 80           | rBV4     | 11835          | 29798         | 2.28%           | 0.455%        |
| 2         | 5.501       | 699           | 713         | 726          | rBV      | 137501         | 400145        | 30.65%          | 6.111%        |
| 3         | 5.659       | 726           | 739         | 756          | rVV      | 235524         | 677165        | 51.87%          | 10.342%       |
| 4         | 6.061       | 793           | 805         | 817          | rBV      | 175371         | 468593        | 35.89%          | 7.157%        |
| 5         | 6.860       | 926           | 936         | 950          | rBV      | 396640         | 947945        | 72.61%          | 14.477%       |
| 6         | 8.713       | 1233          | 1240        | 1252         | rBV      | 832791         | 1305492       | 100.00%         | 19.938%       |
| 7         | 10.110      | 1463          | 1469        | 1486         | rBV      | 761532         | 1065681       | 81.63%          | 16.276%       |
| 8         | 11.134      | 1631          | 1637        | 1647         | rBV      | 596448         | 771818        | 59.12%          | 11.788%       |
| 9         | 12.079      | 1786          | 1792        | 1798         | rBV      | 695564         | 881120        | 67.49%          | 13.457%       |


Sum of corrected areas: 6547757

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX032319\  
Data File : VX008365.D  
Acq On : 23 Mar 2019 21:16  
Operator : JC/SP  
Sample : K1937-15  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BPS1-TT-MW307S-20190314

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X032319W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

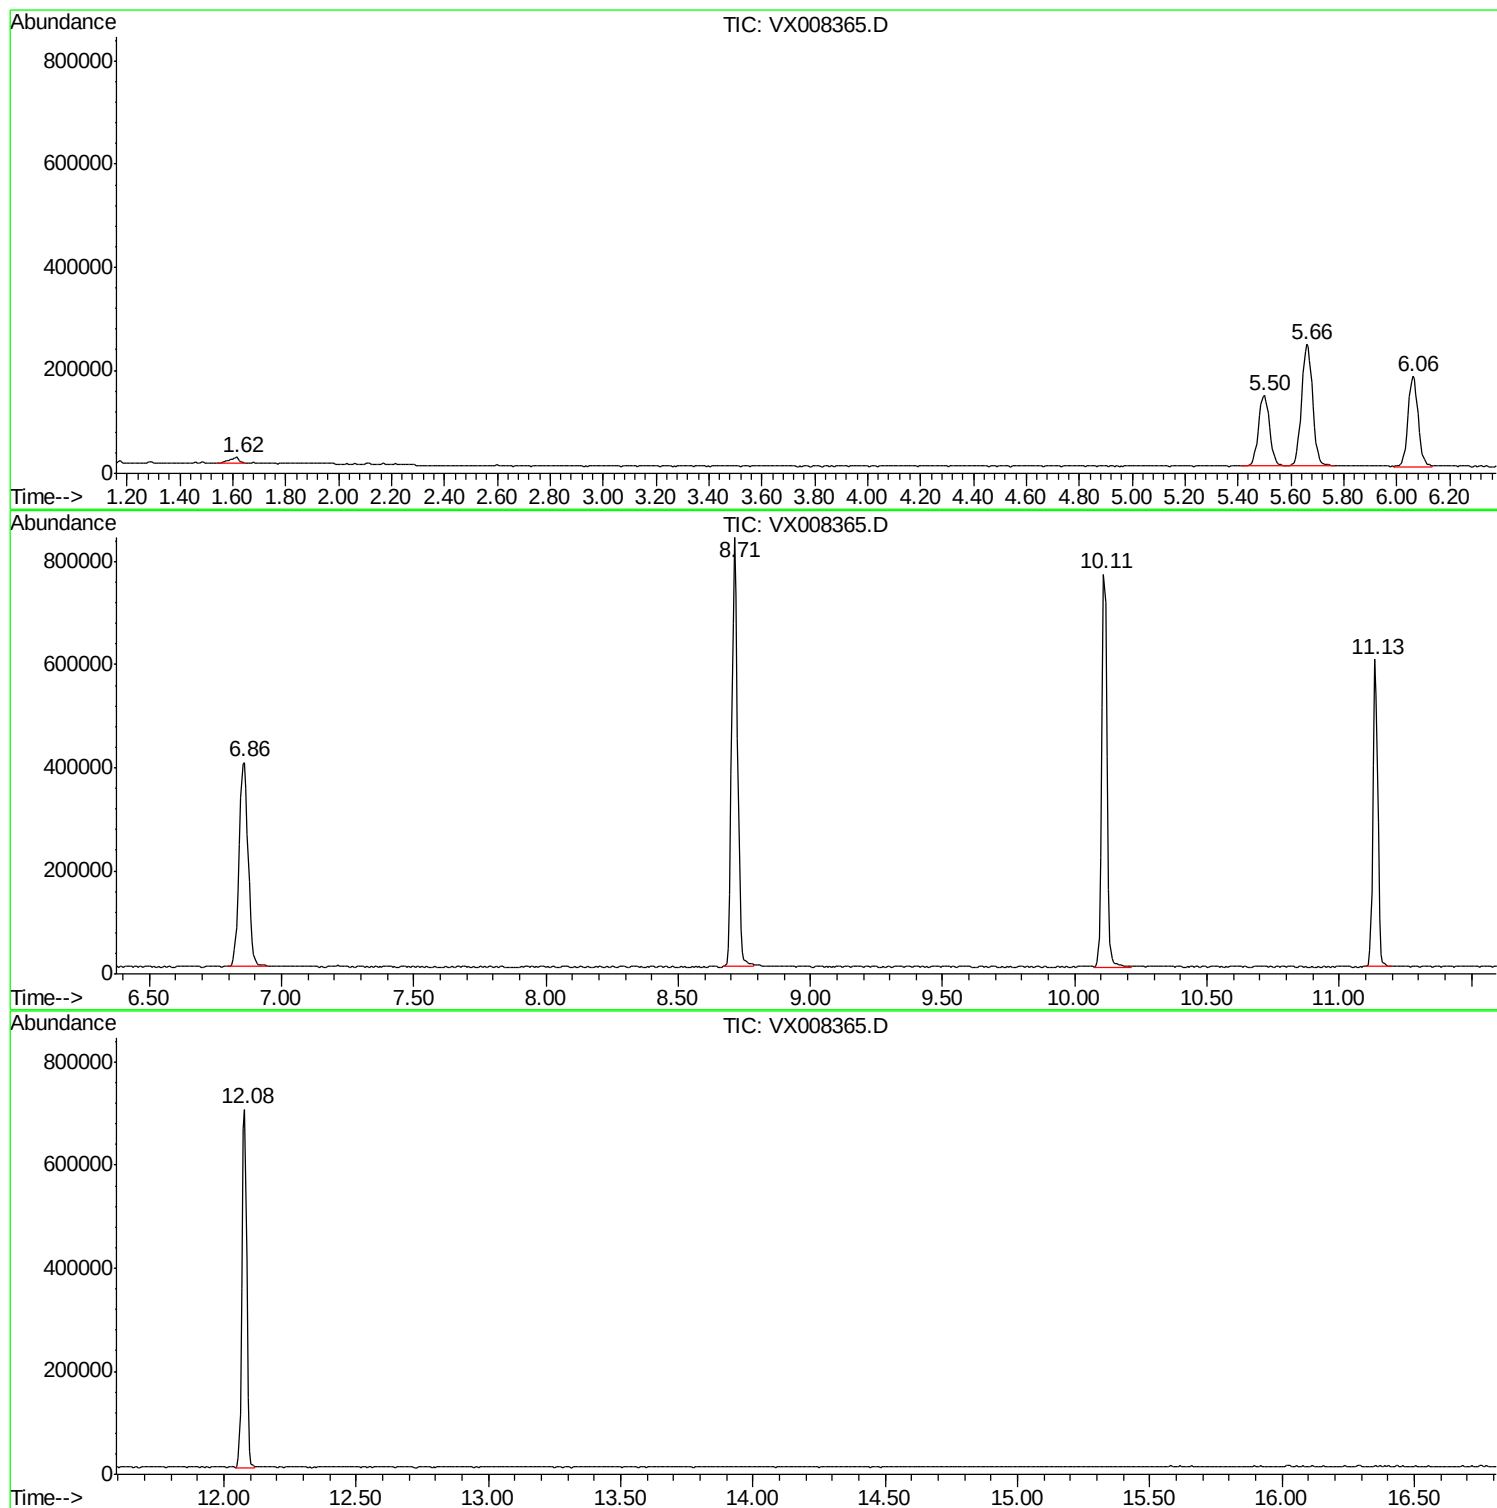

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX032319\  
Data File : VX008365.D  
Acq On : 23 Mar 2019 21:16  
Operator : JC/SP  
Sample : K1937-15  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BPS1-TT-MW307S-20190314

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X032319W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX032319\  
Data File : VX008365.D  
Acq On : 23 Mar 2019 21:16  
Operator : JC/SP  
Sample : K1937-15  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BPS1-TT-MW307S-20190314

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X032319W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | ---Internal Standard--- |
|------------------|----|---------|-------|----------|-------------------------|
|                  |    |         |       |          | # RT Resp Conc          |