


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX032319\
 Data File : VX008344.D
 Acq On : 23 Mar 2019 10:59
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X032319W.M
 Title : SW846 8260
 Last Update : Sat Mar 23 15:27:34 2019

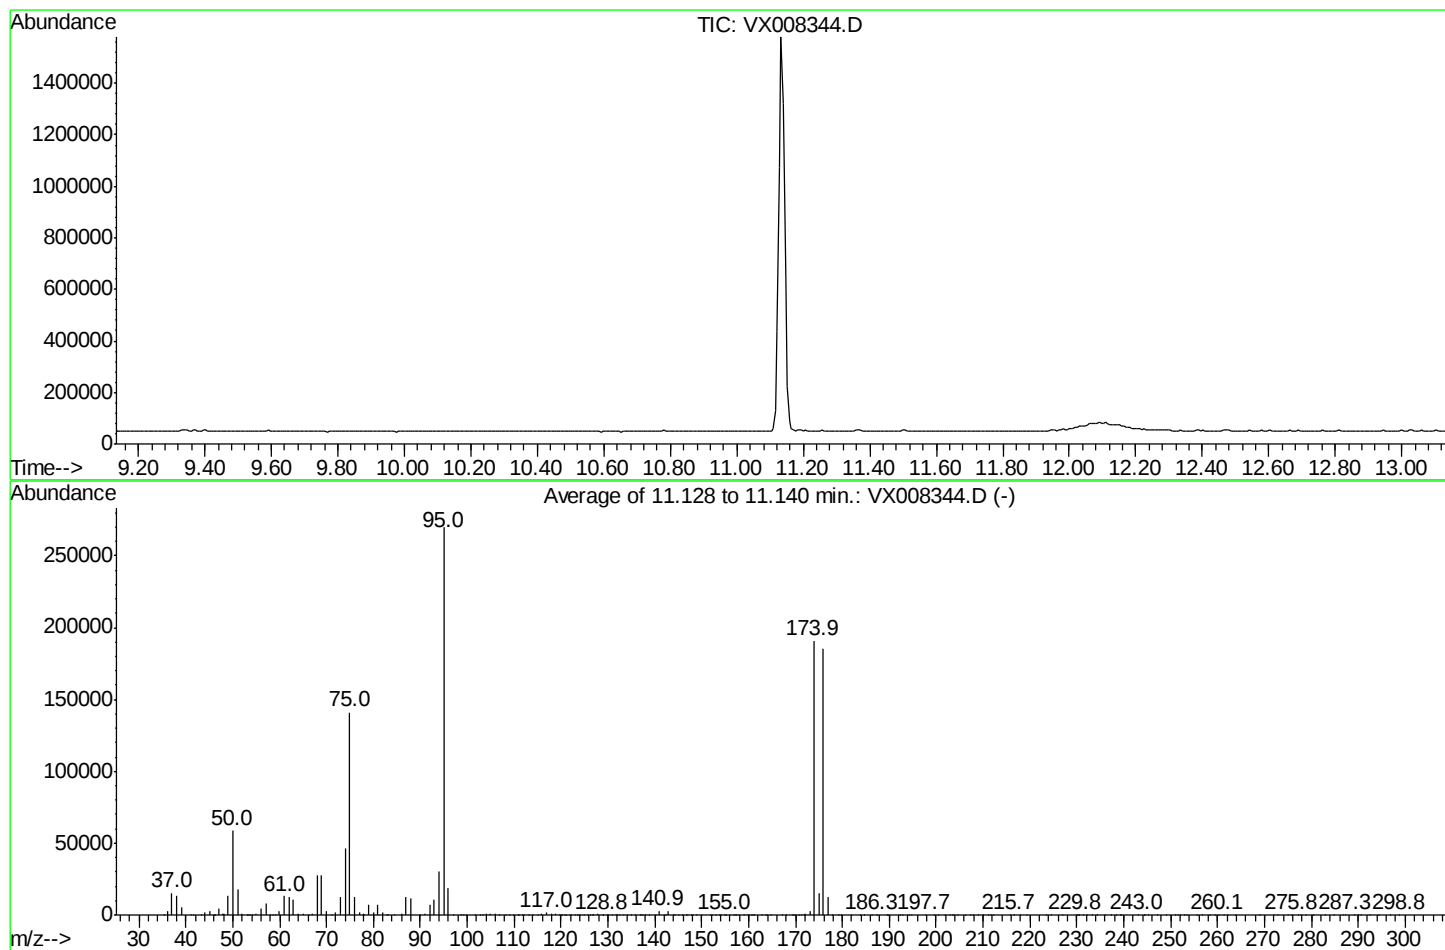

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	58392	PASS
75	95	30	60	52.3	141051	PASS
95	95	100	100	100.0	269791	PASS
96	95	5	9	6.8	18473	PASS
173	174	0.00	2	1.4	2623	PASS
174	95	50	100	70.8	190930	PASS
175	174	5	9	7.8	14855	PASS
176	174	95	101	97.2	185522	PASS
177	176	5	9	6.6	12329	PASS