

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032321\
 Data File : VX021389.D
 Acq On : 23 Mar 2021 16:35
 Operator : JC/MD
 Sample : M1752-13 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 30816

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M

Title : SW846 8260

Signal : TIC: VX021389.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.475	62	66	75	rBV	13690	15741	3.32%	0.570%
2	1.611	78	89	93	rVB8	4517	11070	2.33%	0.401%
3	4.458	566	573	582	rVB	1744	4931	1.04%	0.178%
4	5.464	732	744	761	rBV	56792	162163	34.17%	5.868%
5	5.629	761	772	789	rVV	99191	274487	57.84%	9.933%
6	6.035	828	841	853	rBV	66284	176790	37.26%	6.398%
7	6.829	964	976	987	rBV	148524	352820	74.35%	12.768%
8	6.941	987	995	1005	rVB	65254	149169	31.43%	5.398%
9	7.270	1041	1051	1060	rBV	35241	72534	15.29%	2.625%
10	7.353	1060	1065	1073	rVB3	2747	5323	1.12%	0.193%
11	8.694	1284	1293	1303	rBV	300792	474534	100.00%	17.172%
12	10.094	1525	1531	1547	rVB	290125	399666	84.22%	14.463%
13	11.118	1700	1705	1715	rBV	231428	307802	64.86%	11.139%
14	12.059	1860	1865	1873	rVB	289591	356307	75.09%	12.894%




Sum of corrected areas: 2763337

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032321\
Data File : VX021389.D
Acq On : 23 Mar 2021 16:35
Operator : JC/MD
Sample : M1752-13 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
30816

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

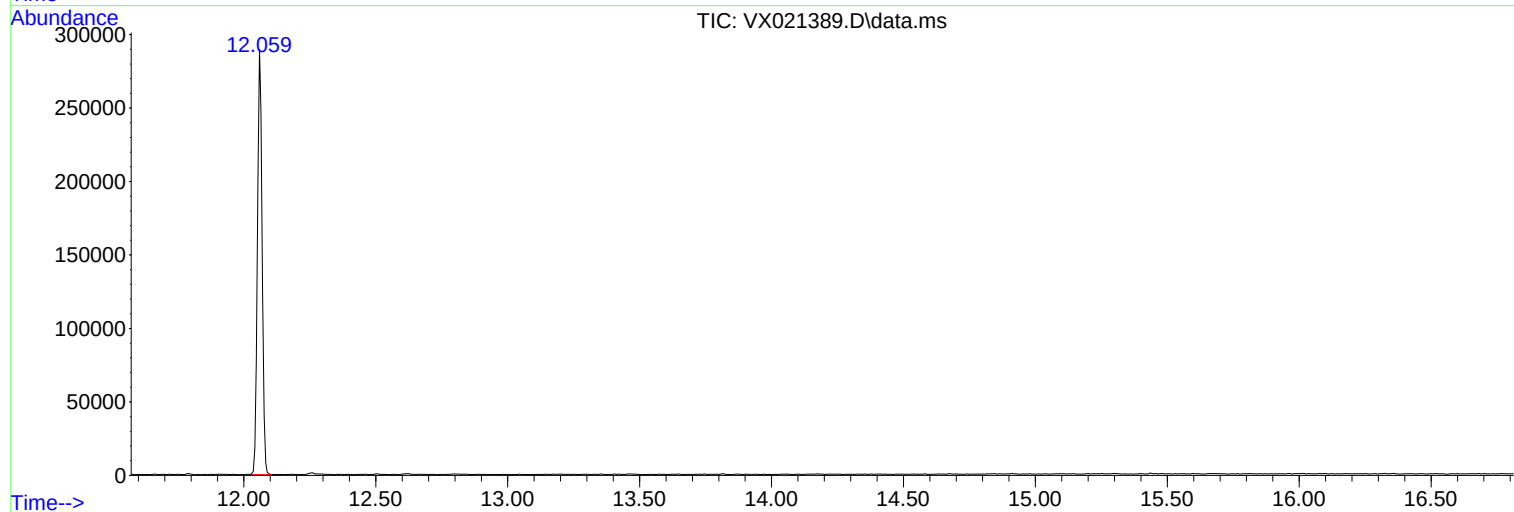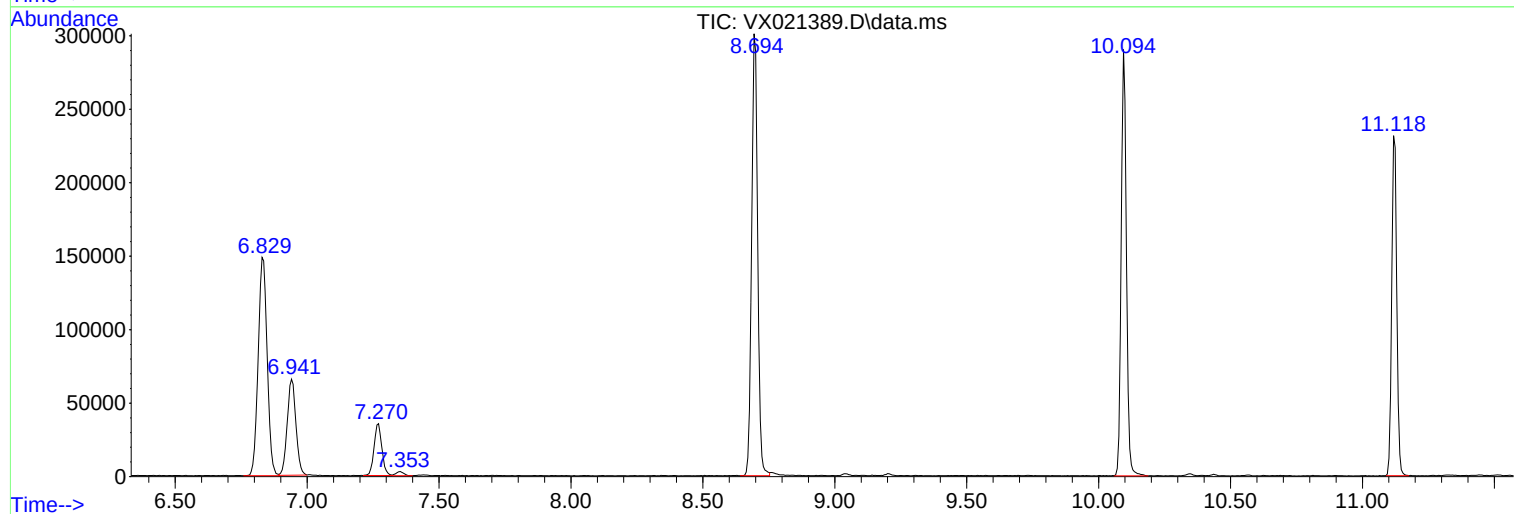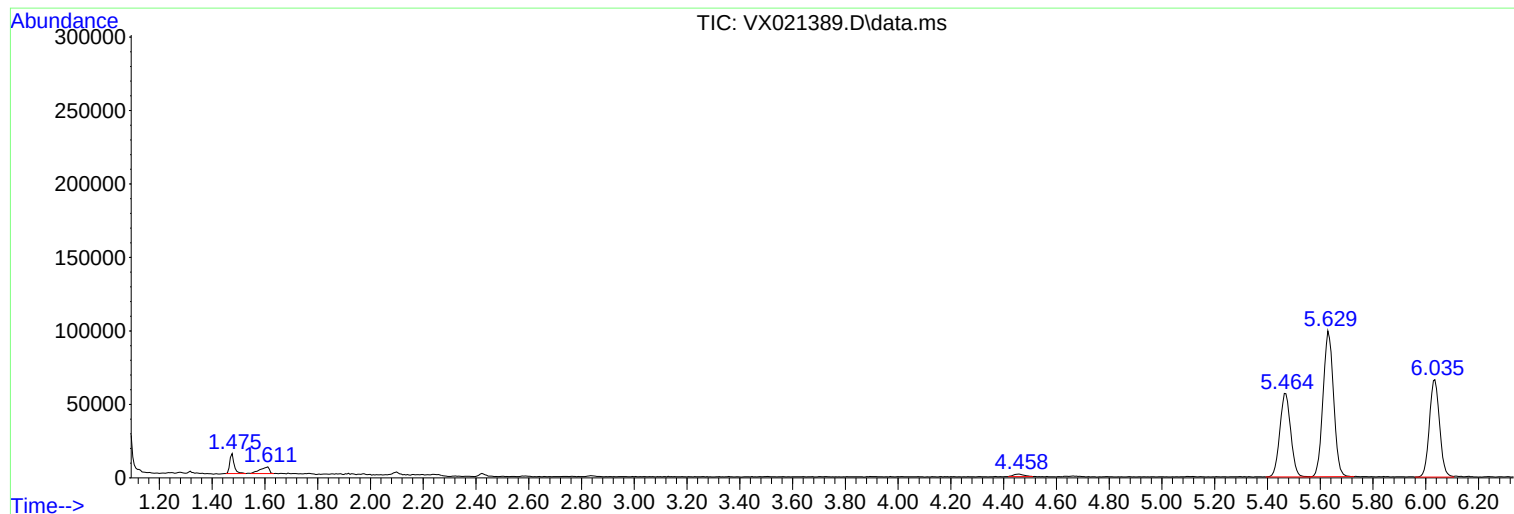

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032321\
Data File : VX021389.D
Acq On : 23 Mar 2021 16:35
Operator : JC/MD
Sample : M1752-13 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
30816










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1,3-Dioxane, 2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.941	21.14 ug/l	149169	1,4-Difluorobenzene	6.829

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1,3-Dioxane, 2-methyl-	102	C5H10O2	000626-68-6	53
2			Oxazolidin-2-one	87	C3H5NO2	000497-25-6	46
3			2-(2-Methoxyethoxy)ethyl acetate	162	C7H14O4	1000351-95-4	42
4			2-[2-[2-[2-[2-[2-[2-[2-[2-(2-...	558	C25H50O13	1000351-91-9	42
5			2-[2-[2-[2-[2-[2-(2-Methoxyethox...	382	C17H34O9	1000351-91-6	42

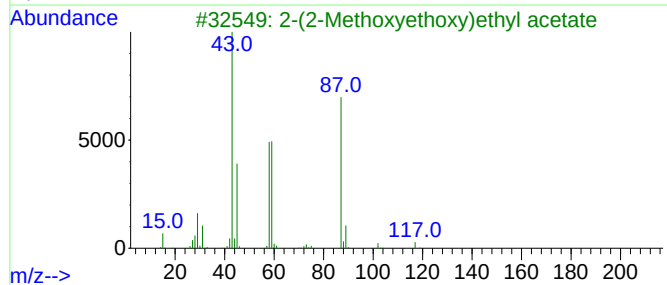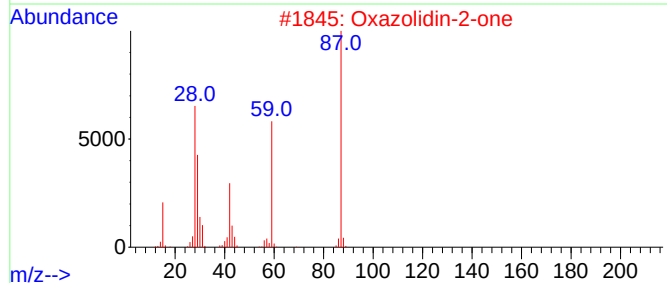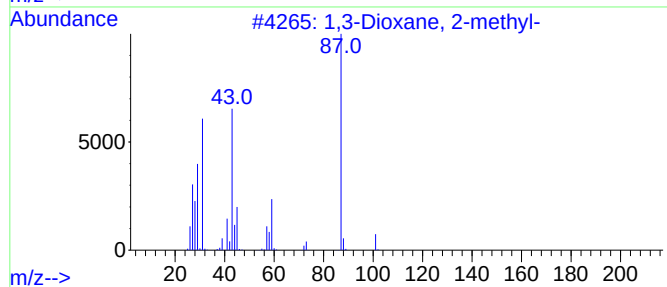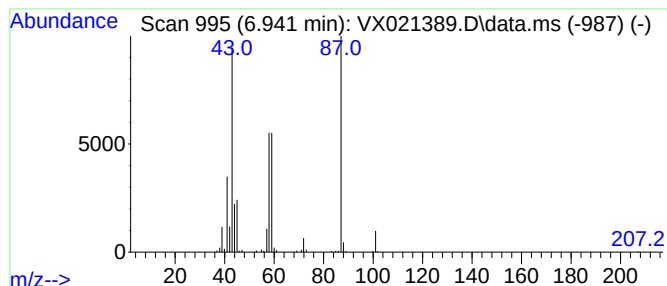

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032321\
Data File : VX021389.D
Acq On : 23 Mar 2021 16:35
Operator : JC/MD
Sample : M1752-13 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
30816










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.270 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.270	10.28 ug/l	72534	1,4-Difluorobenzene	6.829

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		1,3-Dioxane, 2-methyl-	102	C5H10O2	000626-68-6	38
2		Oxazolidin-2-one	87	C3H5NO2	000497-25-6	38
3		1,3-Dioxolane, 2-ethyl-4-methyl-	116	C6H12O2	004359-46-0	28
4		2-(2-Methoxyethoxy)ethyl acetate	162	C7H14O4	1000351-95-4	28
5		Oxirane, (propoxymethyl)-	116	C6H12O2	003126-95-2	25

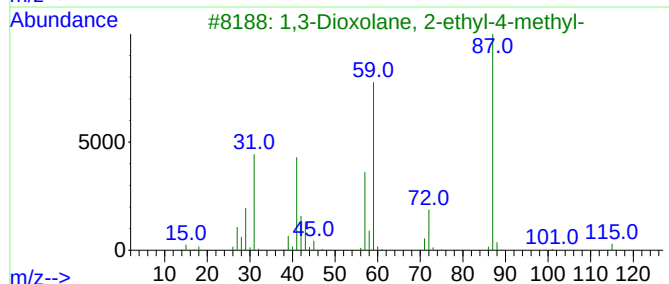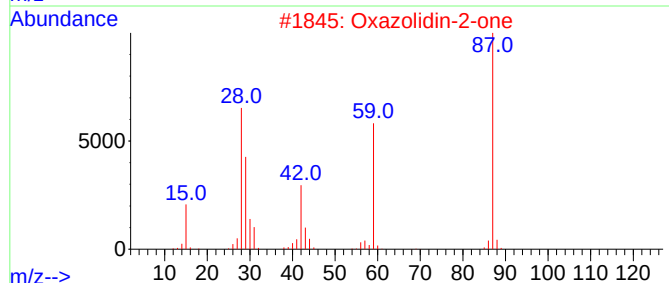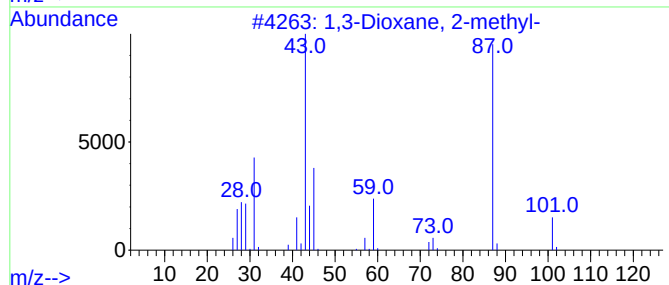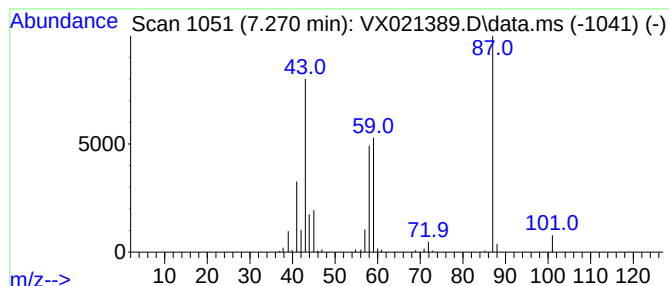

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032321\
Data File : VX021389.D
Acq On : 23 Mar 2021 16:35
Operator : JC/MD
Sample : M1752-13 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
30816

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1,3-Dioxane, 2-...	6.941	21.1	ug/l	149169	2	6.829	352820	50.0
unknown7.270	7.270	10.3	ug/l	72534	2	6.829	352820	50.0