

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032321\
 Data File : VX021406.D
 Acq On : 24 Mar 2021 00:21
 Operator : JC/MD
 Sample : M1735-10 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE132D6-20210315

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M

Title : SW846 8260

Signal : TIC: VX021406.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.652	75	96	99	rBV	8957	44140	6.75%	1.581%
2	2.352	208	215	223	rVB4	5538	11315	1.73%	0.405%
3	5.464	731	744	759	rBV	48349	140976	21.56%	5.050%
4	5.623	759	771	787	rBV	82894	235605	36.03%	8.440%
5	6.029	827	840	851	rBV	59658	154274	23.59%	5.526%
6	6.829	964	976	990	rBV	129736	304583	46.58%	10.911%
7	7.188	1027	1037	1054	rBV	302891	653961	100.00%	23.427%
8	8.694	1285	1293	1302	rBV	264084	409033	62.55%	14.653%
9	10.094	1524	1531	1546	rBV	246559	332809	50.89%	11.922%
10	11.118	1700	1705	1716	rVB	185581	241318	36.90%	8.645%
11	12.059	1860	1865	1872	rVB	213799	263522	40.30%	9.440%




Sum of corrected areas: 2791536

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032321\
Data File : VX021406.D
Acq On : 24 Mar 2021 00:21
Operator : JC/MD
Sample : M1735-10 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D6-20210315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

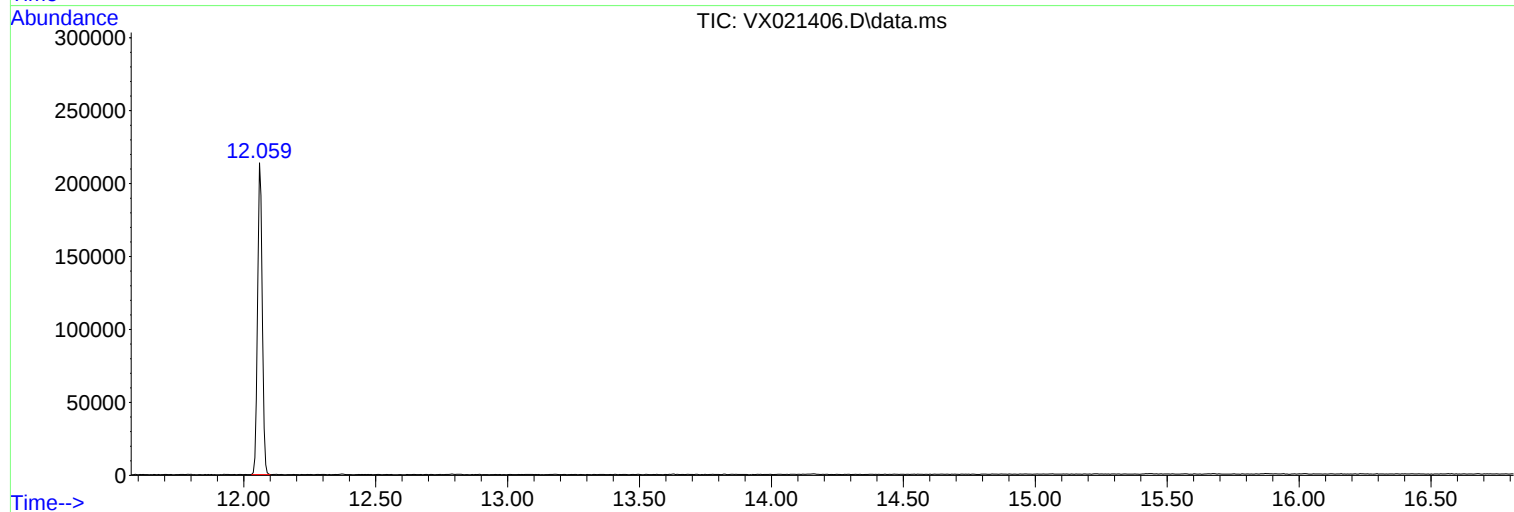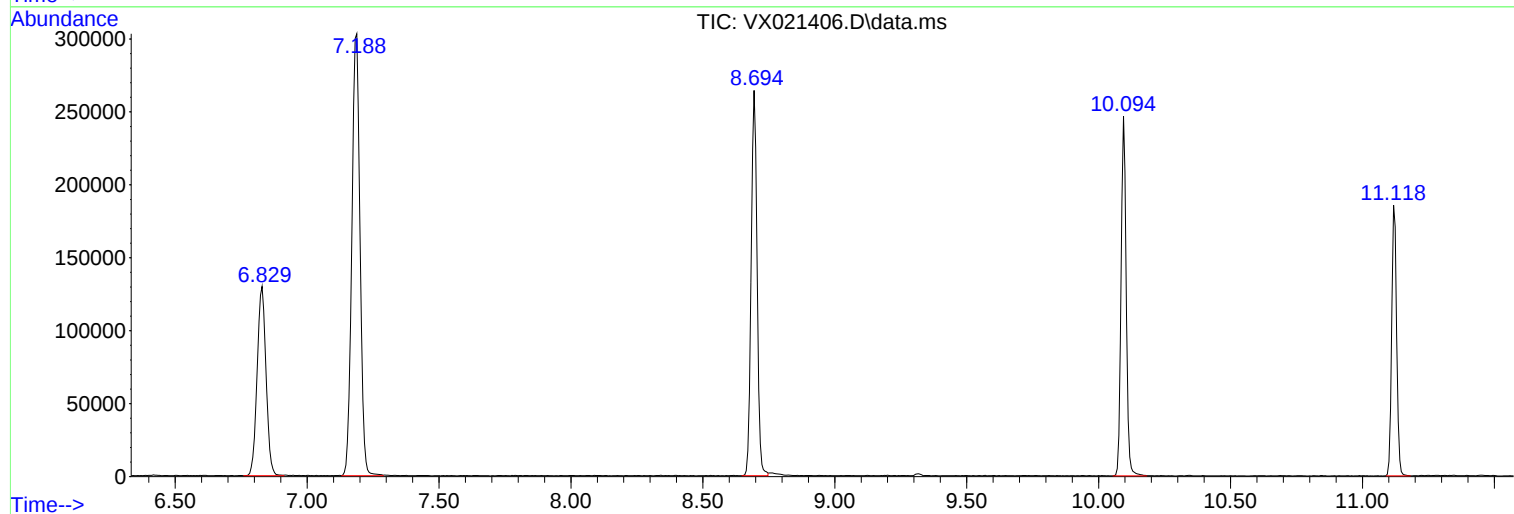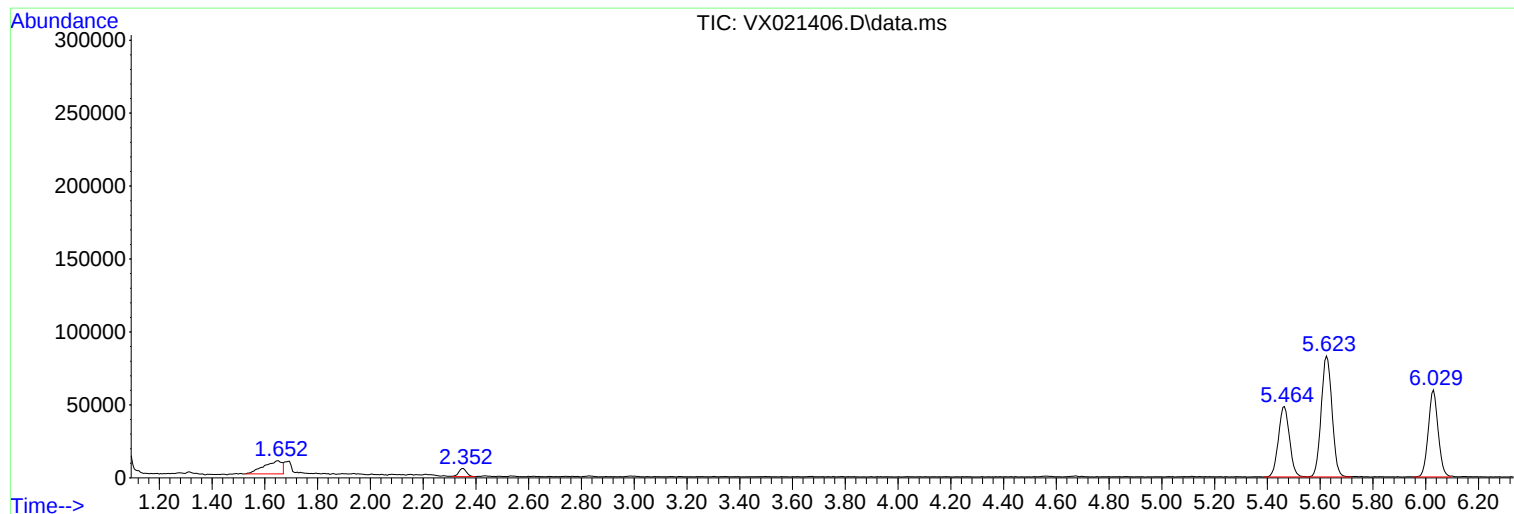

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032321\
Data File : VX021406.D
Acq On : 24 Mar 2021 00:21
Operator : JC/MD
Sample : M1735-10 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D6-20210315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032321\
Data File : VX021406.D
Acq On : 24 Mar 2021 00:21
Operator : JC/MD
Sample : M1735-10 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D6-20210315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
