

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032321\
 Data File : VX021416.D
 Acq On : 24 Mar 2021 04:15
 Operator : JC/MD
 Sample : M1774-02 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 30806

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M

Title : SW846 8260

Signal : TIC: VX021416.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	27	32	36	rBV2	4013	4464	1.03%	0.192%
2	1.605	78	88	94	rVB8	4616	11589	2.67%	0.500%
3	2.417	218	226	234	rBV	20045	34771	8.02%	1.499%
4	5.464	732	744	760	rVB2	52819	149035	34.38%	6.426%
5	5.629	760	772	783	rBV	88211	242409	55.92%	10.453%
6	6.029	829	840	855	rBV2	61970	162065	37.39%	6.988%
7	6.829	963	976	989	rBV	134727	317945	73.35%	13.710%
8	8.694	1286	1293	1311	rBV	280558	433492	100.00%	18.692%
9	10.094	1525	1531	1548	rVB	268757	370174	85.39%	15.962%
10	11.118	1700	1705	1715	rBV	217419	278628	64.28%	12.014%
11	12.059	1859	1865	1874	rVB	258510	314563	72.56%	13.564%




Sum of corrected areas: 2319135

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032321\
Data File : VX021416.D
Acq On : 24 Mar 2021 04:15
Operator : JC/MD
Sample : M1774-02 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
30806

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

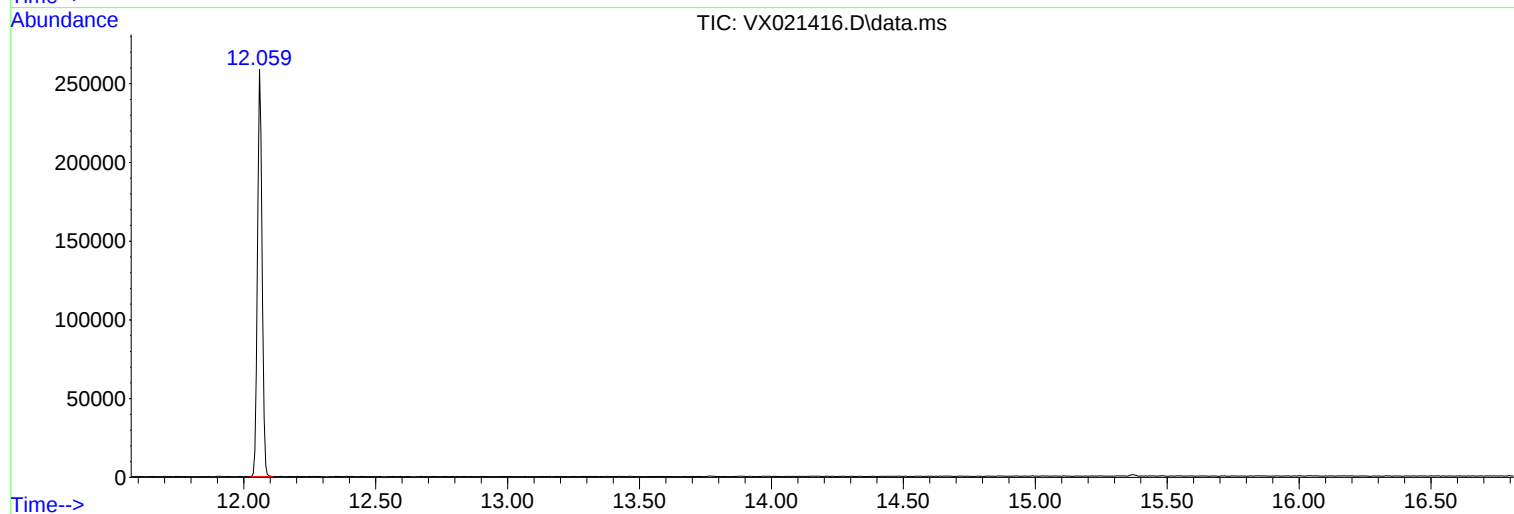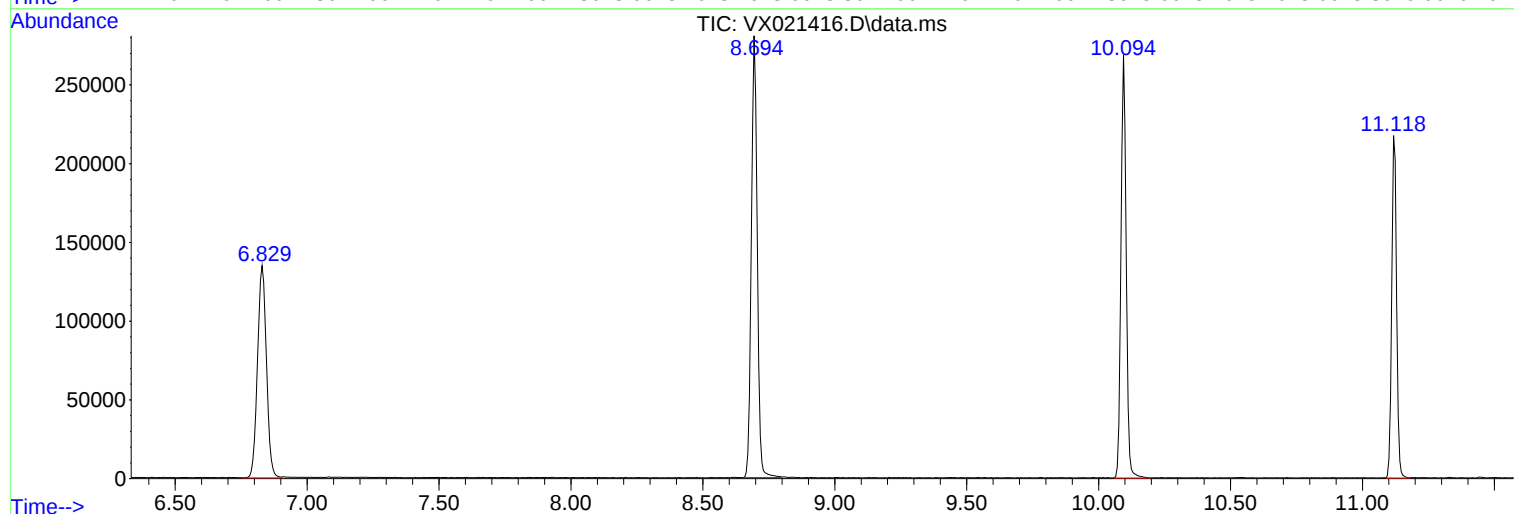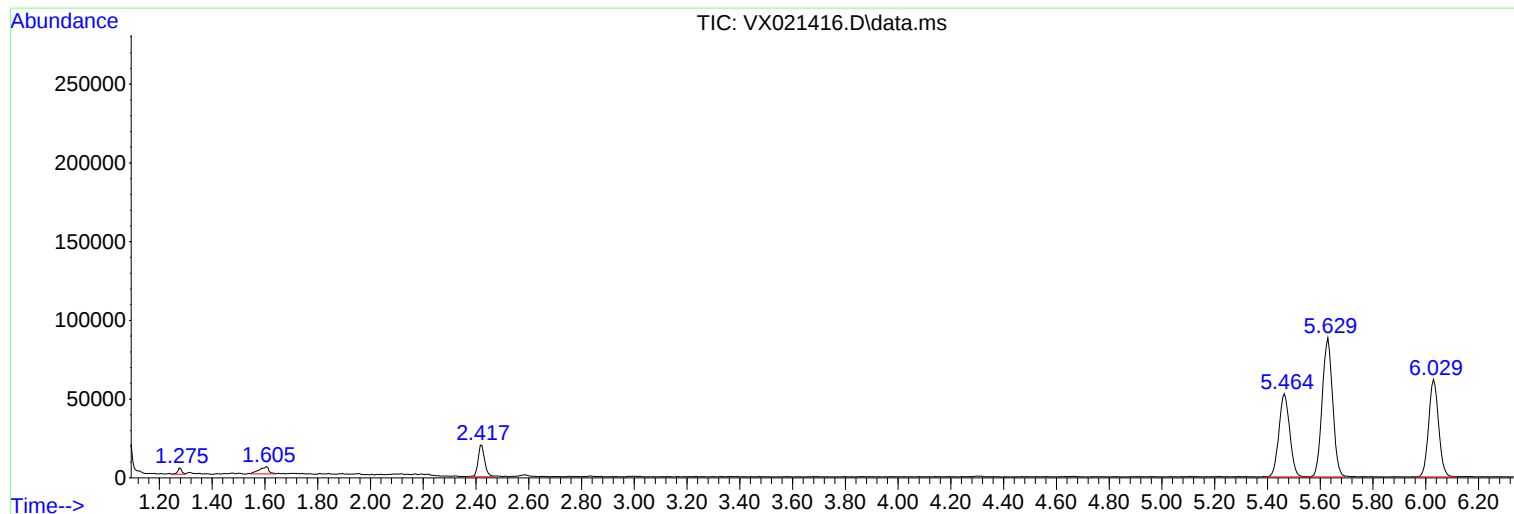

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032321\
Data File : VX021416.D
Acq On : 24 Mar 2021 04:15
Operator : JC/MD
Sample : M1774-02 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
30806

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032321\
Data File : VX021416.D
Acq On : 24 Mar 2021 04:15
Operator : JC/MD
Sample : M1774-02 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
30806

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------