

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032321\
 Data File : VX021417.D
 Acq On : 24 Mar 2021 04:38
 Operator : JC/MD
 Sample : M1774-01 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 41736

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M

Title : SW846 8260

Signal : TIC: VX021417.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.475	61	66	79	rBV	390693	460219	100.00%	17.143%
2	2.093	166	171	177	rBV	3304	5869	1.28%	0.219%
3	4.311	537	548	554	rBV5	1598	5118	1.11%	0.191%
4	5.464	733	744	758	rBV	52249	148749	32.32%	5.541%
5	5.629	761	772	787	rBV	85798	241244	52.42%	8.986%
6	6.029	828	840	854	rBV	61457	159792	34.72%	5.952%
7	6.829	966	976	994	rBV	135854	316129	68.69%	11.776%
8	8.694	1284	1293	1303	rBV	271968	424503	92.24%	15.813%
9	10.094	1524	1531	1546	rBV	262202	360866	78.41%	13.442%
10	11.118	1700	1705	1717	rVB	206885	266021	57.80%	9.909%
11	12.059	1858	1865	1874	rVB	243005	296092	64.34%	11.029%




Sum of corrected areas: 2684602

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032321\
Data File : VX021417.D
Acq On : 24 Mar 2021 04:38
Operator : JC/MD
Sample : M1774-01 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
41736

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

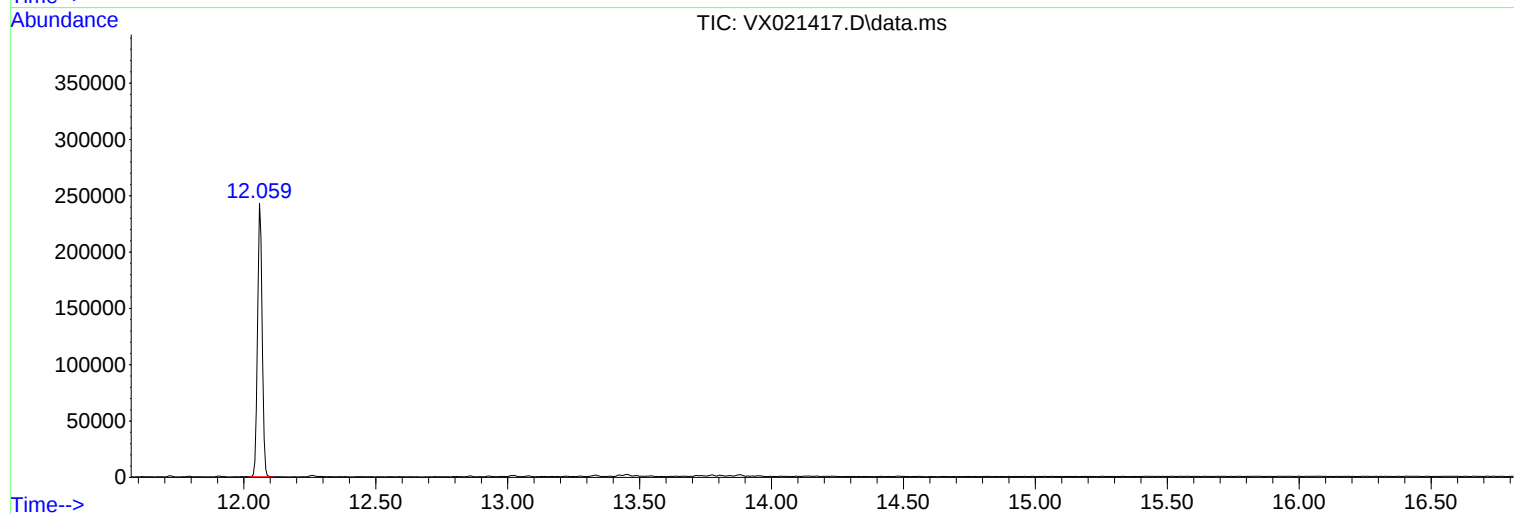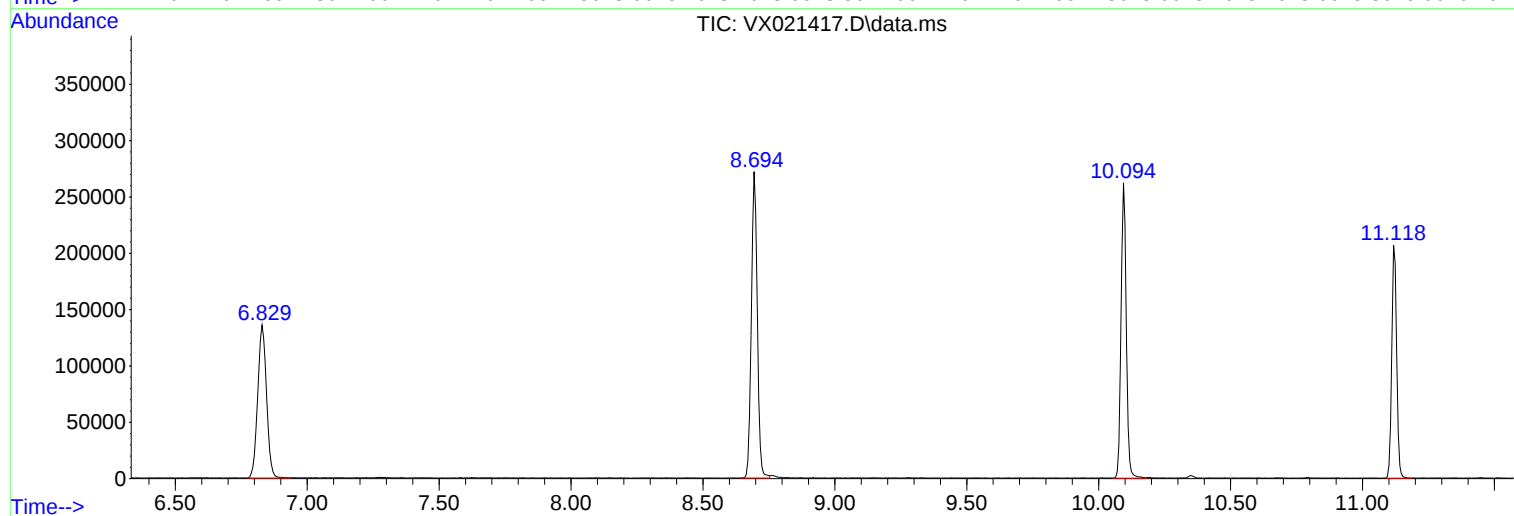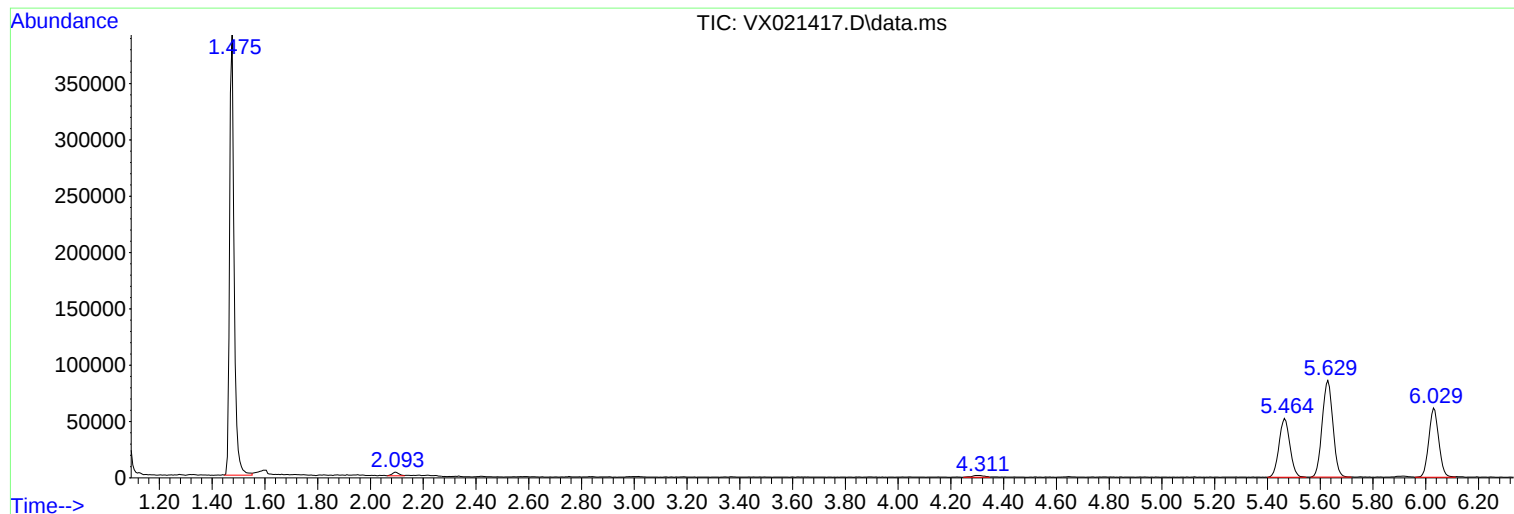

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032321\
Data File : VX021417.D
Acq On : 24 Mar 2021 04:38
Operator : JC/MD
Sample : M1774-01 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
41736

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032321\
Data File : VX021417.D
Acq On : 24 Mar 2021 04:38
Operator : JC/MD
Sample : M1774-01 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
41736

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
