
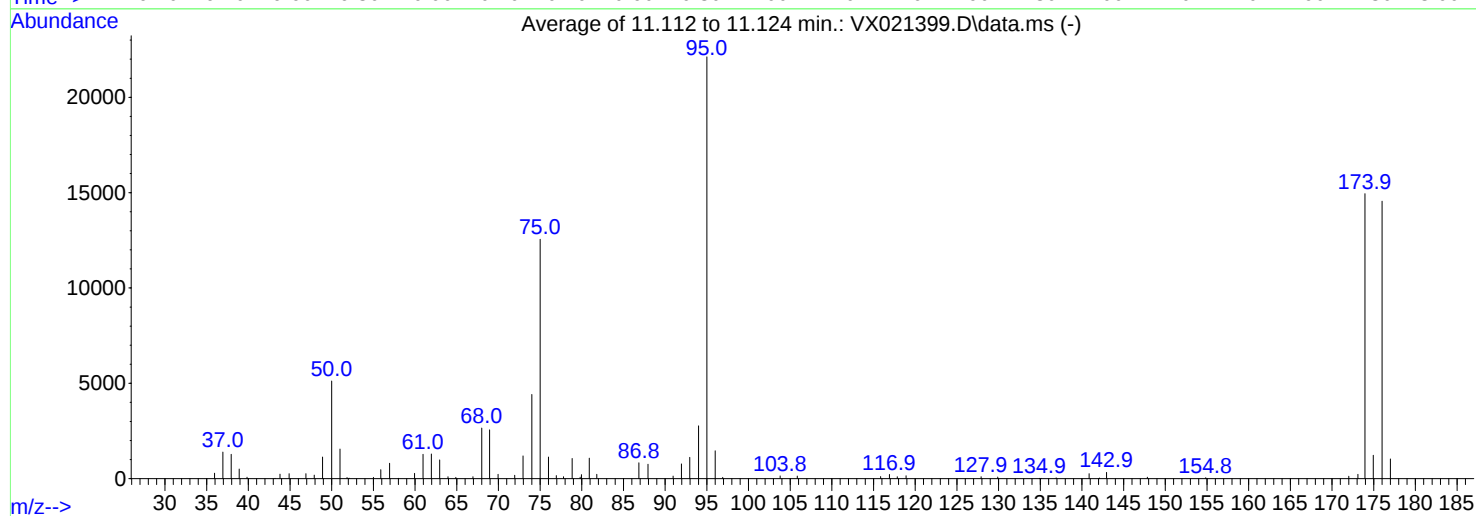


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032321\
Data File : VX021399.D
Acq On : 23 Mar 2021 20:50
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031621W.M
Title : SW846 8260
Last Update : Tue Mar 16 14:00:21 2021

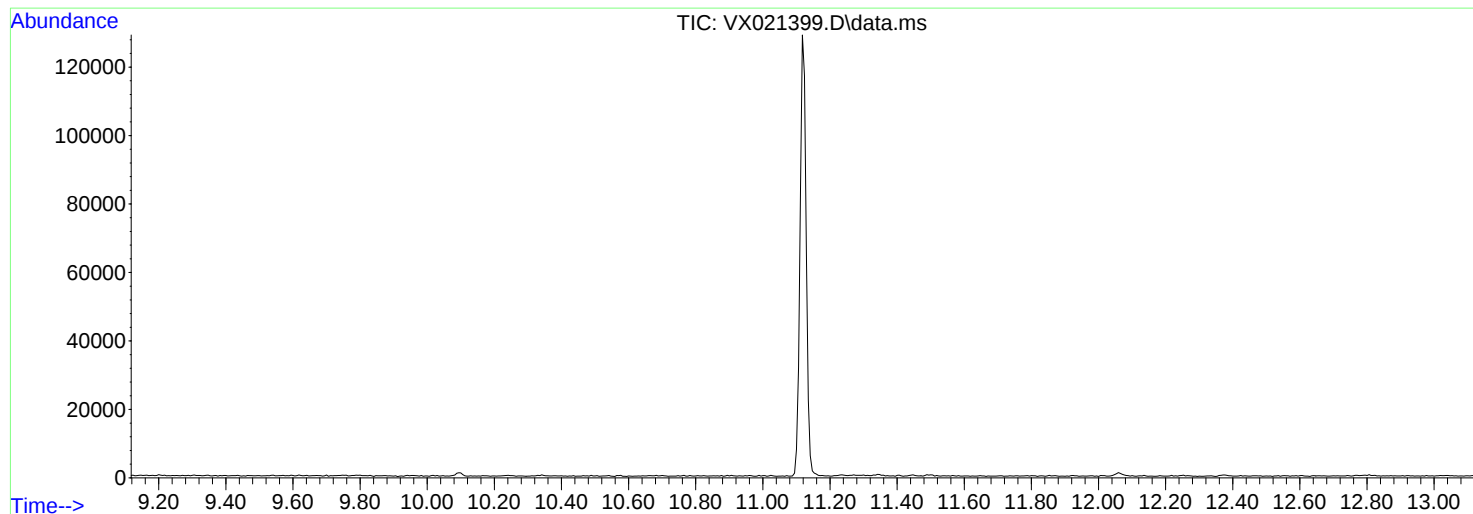

AutoFind: Scans 1704, 1705, 1706; Background Corrected with Scan 1698

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.2	5123	PASS
75	95	30	60	56.7	12552	PASS
95	95	100	100	100.0	22123	PASS
96	95	5	9	6.6	1459	PASS
173	174	0.00	2	1.5	226	PASS
174	95	50	100	67.6	14948	PASS
175	174	5	9	8.2	1227	PASS
176	174	95	101	97.4	14554	PASS
177	176	5	9	7.1	1034	PASS