

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032322\
 Data File : VX027670.D
 Acq On : 23 Mar 2022 16:14
 Operator : JC/MD
 Sample : N1908-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WC-14A-2

Quant Time: Mar 23 17:28:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 17 15:02:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	359325	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	582104	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	549812	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	255572	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	195898	44.255	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	88.520%		
35) Dibromofluoromethane	5.391	113	186776	49.871	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	99.740%		
50) Toluene-d8	8.653	98	683759	48.247	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	96.500%		
62) 4-Bromofluorobenzene	11.079	95	282251	54.185	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	108.380%		
Target Compounds					Qvalue	
5) Bromomethane	1.605	94	755	Below Cal		90
6) Chloroethane	1.685	64	1003	0.462 ug/l #		53
11) Tert butyl alcohol	2.947	59	1824	2.162 ug/l #		72
16) Acetone	2.380	43	28030	15.535 ug/l		97
18) Methyl Acetate	2.709	43	17046	3.942 ug/l		98
20) Methylene Chloride	2.788	84	8847	2.281 ug/l		98
25) 2-Butanone	4.568	43	9522	3.508 ug/l		95
29) Tetrahydrofuran	5.032	42	402	0.231 ug/l #		29
31) Cyclohexane	5.464	56	2954	0.537 ug/l		93
36) 1,1-Dichloropropene	5.556	75	23375	4.567 ug/l #		50
37) Ethyl Acetate	4.568	43	9522	1.867 ug/l #		65
38) Carbon Tetrachloride	5.550	117	34085	5.821 ug/l #		15
39) Methylcyclohexane	7.385	83	3819	0.593 ug/l		99
43) Isopropyl Acetate	6.342	43	25911	3.157 ug/l		98
48) Methyl methacrylate	7.598	41	8731	2.149 ug/l #		7
49) 1,4-Dioxane	7.793	88	375	3.594 ug/l #		1
51) 4-Methyl-2-Pentanone	8.549	43	76558	14.612 ug/l #		46
52) Toluene	8.720	92	2155	0.219 ug/l		80
54) cis-1,3-Dichloropropene	8.549	75	39456	6.566 ug/l #		67
57) 1,3-Dichloropropane	9.482	76	24568	3.777 ug/l #		43
59) 2-Hexanone	9.482	43	276506	68.522 ug/l #		45
67) Ethyl Benzene	10.195	91	4269	0.221 ug/l		96
68) m/p-Xylenes	10.305	106	4298	0.564 ug/l		93
69) o-Xylene	10.646	106	11246	1.520 ug/l		100
76) 1,2,3-Trichloropropane	11.079	75	132145	24.720 ug/l #		38
80) 1,3,5-Trimethylbenzene	11.451	105	12510	0.798 ug/l		100
81) trans-1,4-Dichloro-2-b...	11.079	75	132145	75.075 ug/l #		15
84) 1,2,4-Trimethylbenzene	11.756	105	29968	1.918 ug/l		98
89) n-Butylbenzene	12.323	91	2722	0.202 ug/l #		19
95) Naphthalene	13.780	128	45221	2.553 ug/l		98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032322\
Data File : VX027670.D
Acq On : 23 Mar 2022 16:14
Operator : JC/MD
Sample : N1908-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WC-14A-2

Quant Time: Mar 23 17:28:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260
QLast Update : Thu Mar 17 15:02:59 2022
Response via : Initial Calibration



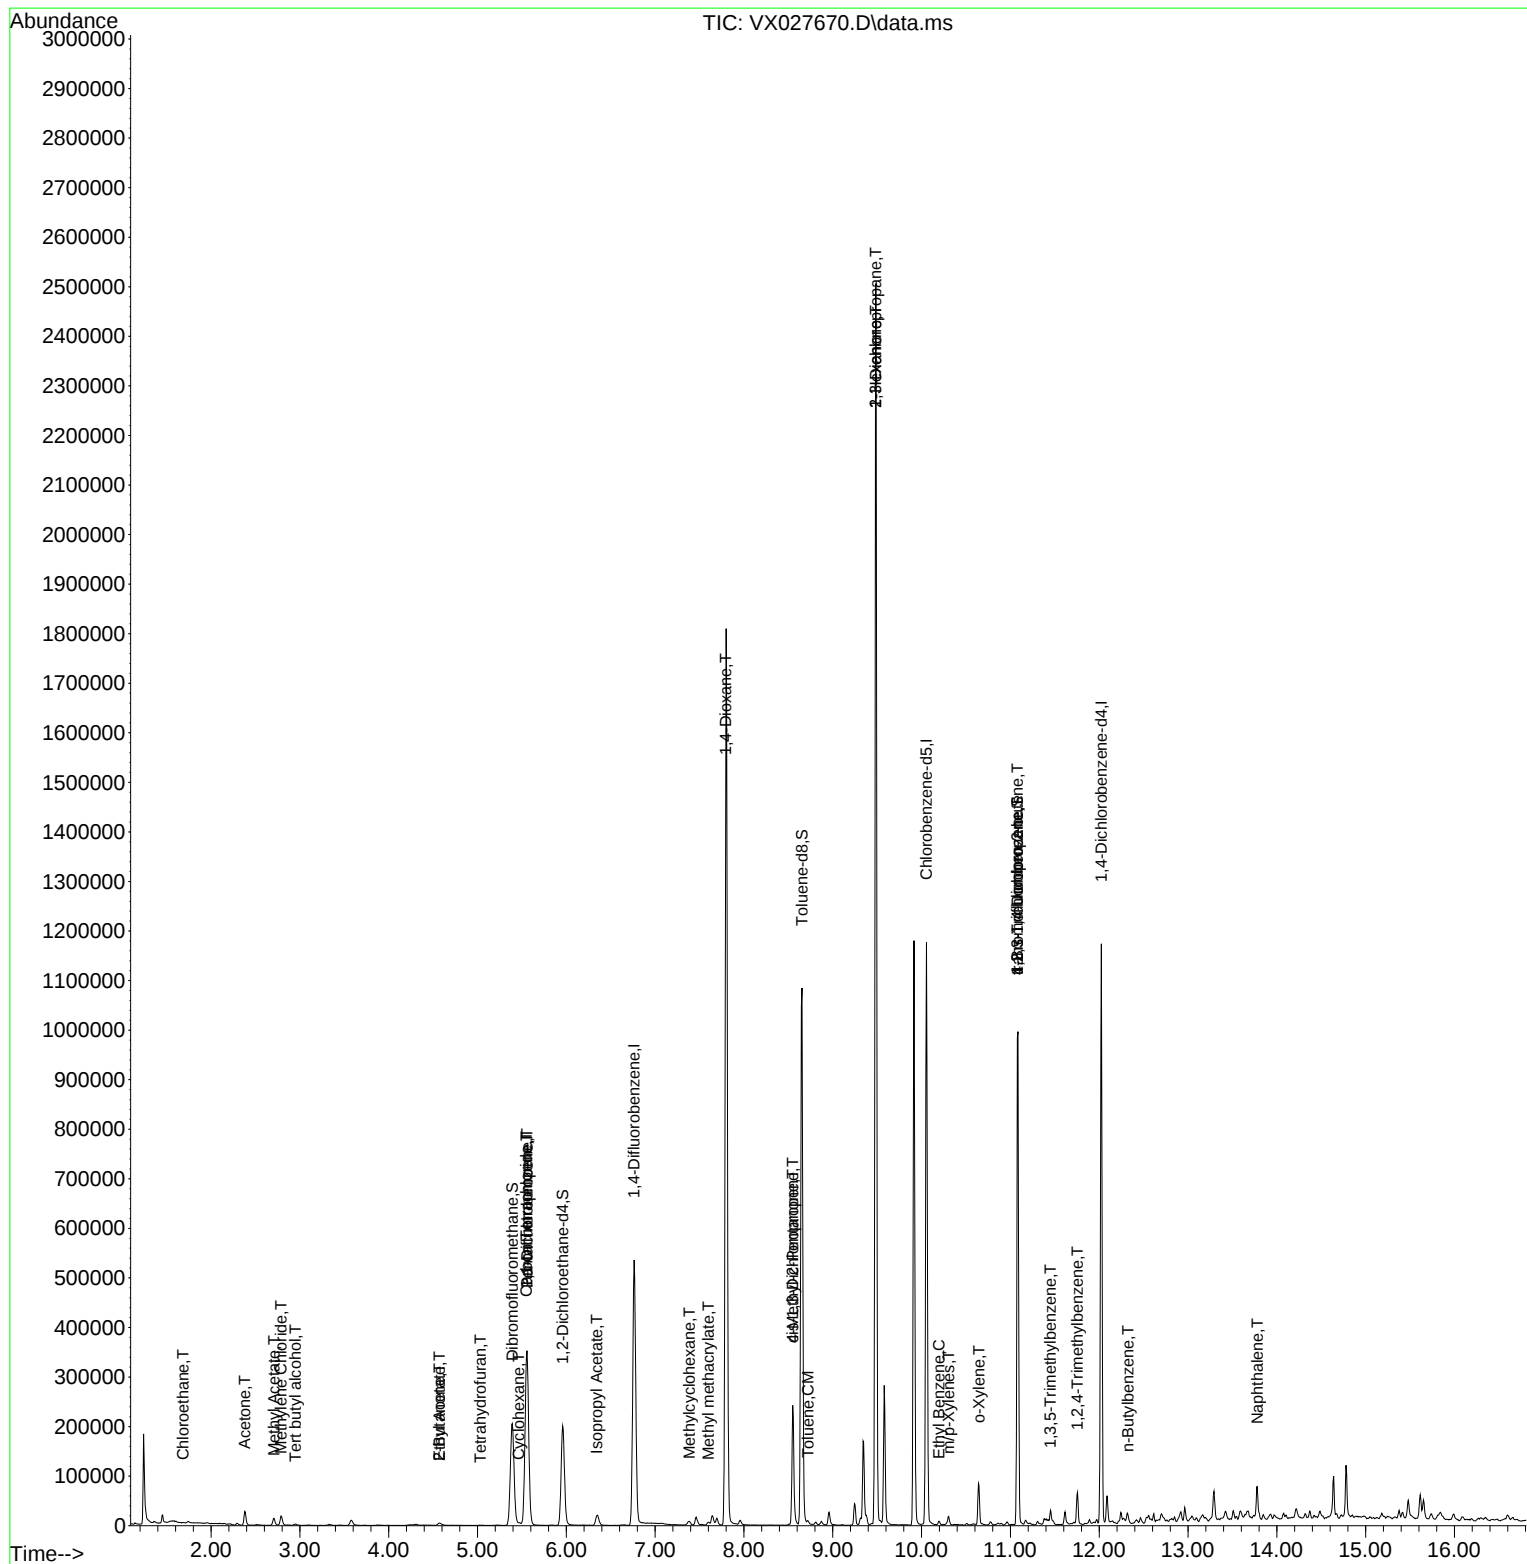




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX027670.D
Acq: 23 Mar 2022 16:14




Instrument :
MSVOA_X
ClientSampleId :
WC-14A-2


Tgt Ion:168 Resp: 359325
Ion Ratio Lower Upper
168 100
99 53.4 41.7 62.5

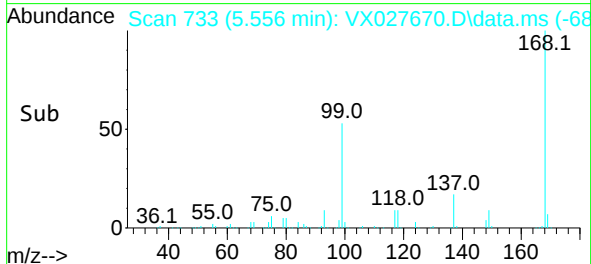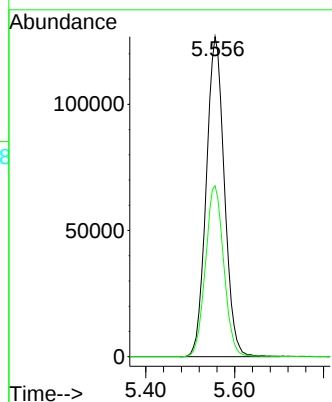

#5
Bromomethane
Concen: Below Cal
RT: 1.605 min Scan# 85
Delta R.T. 0.006 min
Lab File: VX027670.D
Acq: 23 Mar 2022 16:14

Tgt Ion: 94 Resp: 755
Ion Ratio Lower Upper
94 100
96 84.6 75.3 112.9


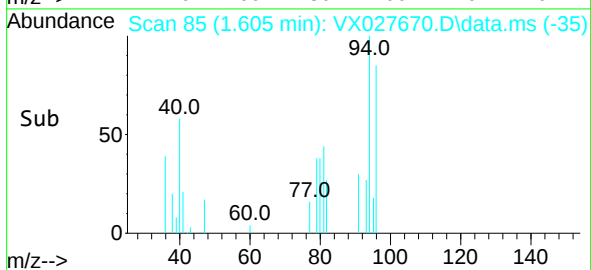
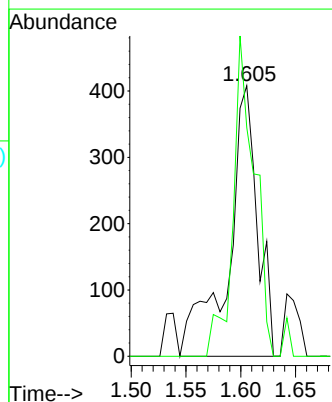
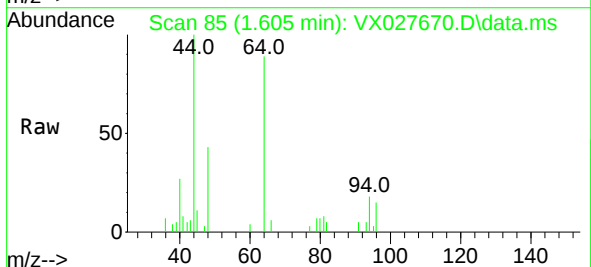


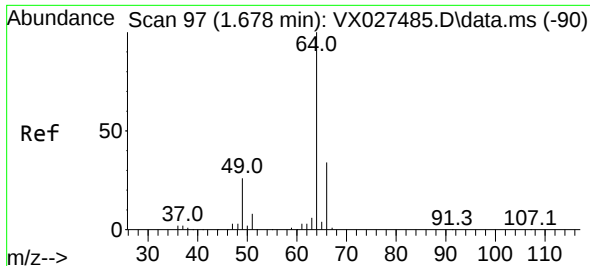

#6
Chloroethane
Concen: 0.462 ug/l
RT: 1.685 min Scan# 91
Delta R.T. 0.006 min
Lab File: VX027670.D
Acq: 23 Mar 2022 16:14




Instrument :
MSVOA_X
ClientSampleId :
WC-14A-2


Tgt Ion: 64 Resp: 1003
Ion Ratio Lower Upper
64 100
66 5.4 25.3 37.9#

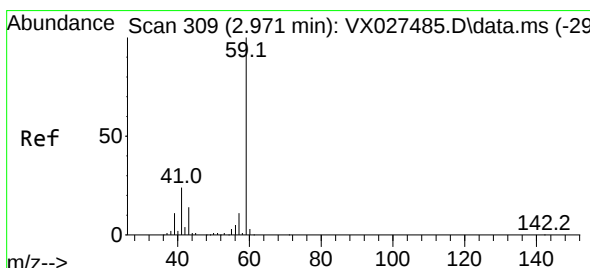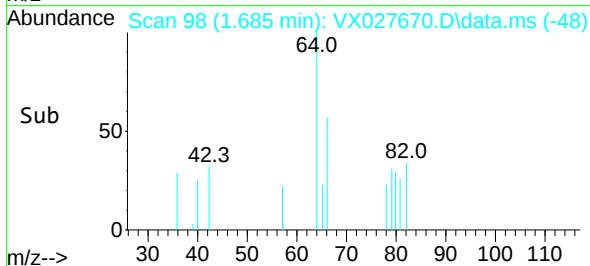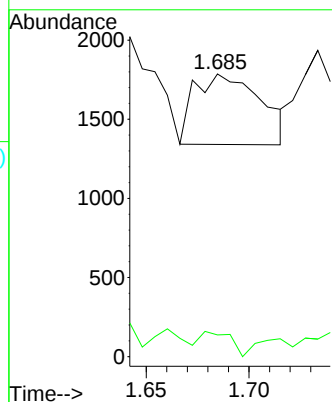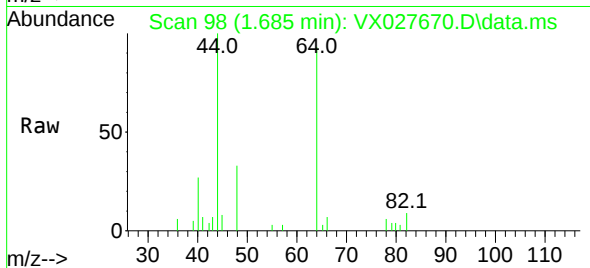

#11
Tert butyl alcohol
Concen: 2.162 ug/l
RT: 2.947 min Scan# 305
Delta R.T. -0.024 min
Lab File: VX027670.D
Acq: 23 Mar 2022 16:14

Tgt Ion: 59 Resp: 1824
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#


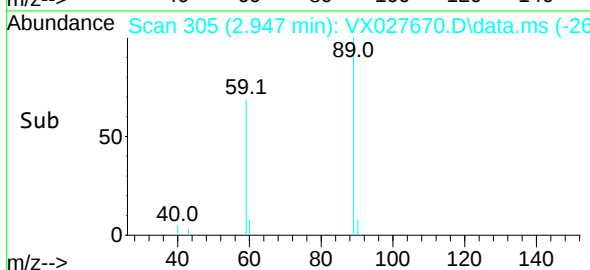

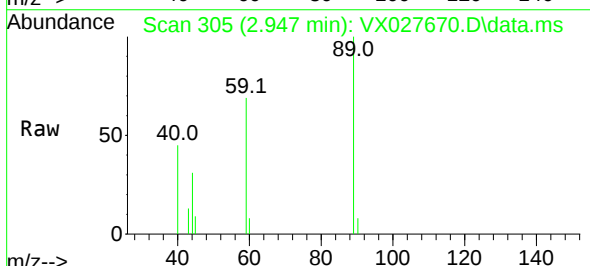




#16
Acetone
Concen: 15.535 ug/l
RT: 2.380 min Scan# 212
Delta R.T. 0.000 min
Lab File: VX027670.D
Acq: 23 Mar 2022 16:14




Instrument :
MSVOA_X
ClientSampleId :
WC-14A-2


Tgt Ion: 43 Resp: 28030
Ion Ratio Lower Upper
43 100
58 34.4 28.8 43.2

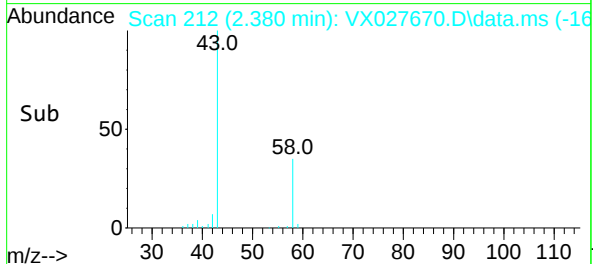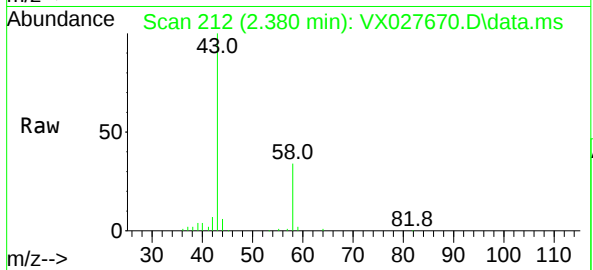

#18
Methyl Acetate
Concen: 3.942 ug/l
RT: 2.709 min Scan# 266
Delta R.T. 0.000 min
Lab File: VX027670.D
Acq: 23 Mar 2022 16:14

Tgt Ion: 43 Resp: 17046
Ion Ratio Lower Upper
43 100
74 27.5 22.8 34.2




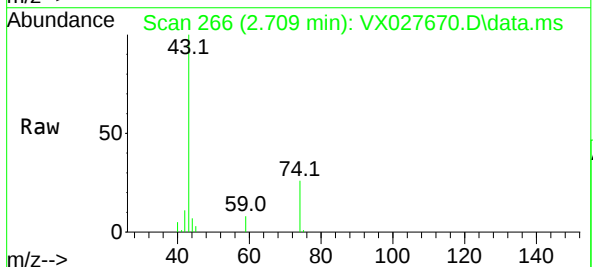




#20
Methylene Chloride
Concen: 2.281 ug/l
RT: 2.788 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX027670.D
Acq: 23 Mar 2022 16:14




Instrument :
MSVOA_X
ClientSampleId :
WC-14A-2


Tgt Ion:	84	Resp:	8847
Ion	Ratio	Lower	Upper
84	100		
49	106.8	85.5	128.3
51	31.1	26.6	39.8
86	62.1	51.5	77.3

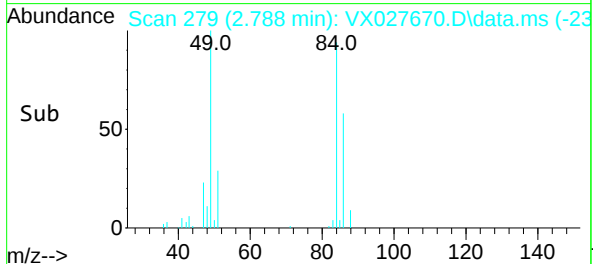

#25
2-Butanone
Concen: 3.508 ug/l
RT: 4.568 min Scan# 571
Delta R.T. 0.006 min
Lab File: VX027670.D
Acq: 23 Mar 2022 16:14

Tgt Ion:	43	Resp:	9522
Ion	Ratio	Lower	Upper
43	100		
72	27.8	24.4	36.6

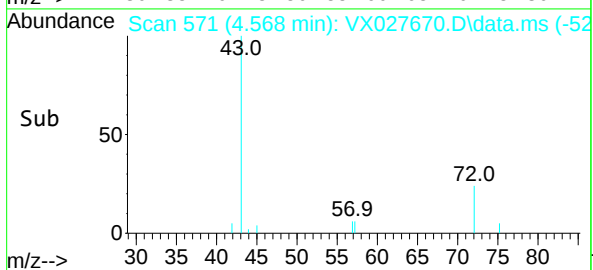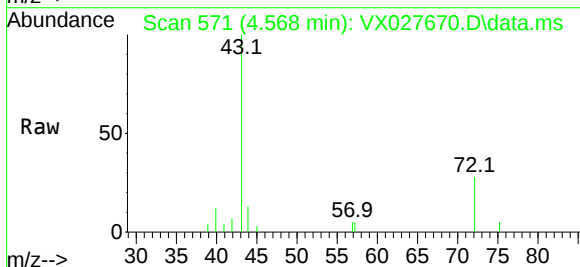



#29

Tetrahydrofuran

Concen: 0.231 ug/l

RT: 5.032 min Scan# 64

Delta R.T. 0.025 min

Lab File: VX027670.D

Acq: 23 Mar 2022 16:14

Instrument :

MSVOA_X

ClientSampleId :

WC-14A-2





Tgt Ion: 42 Resp: 402

Ion Ratio Lower Upper

42 100

72 5.2 44.1 66.1#

71 0.0 40.5 60.7#

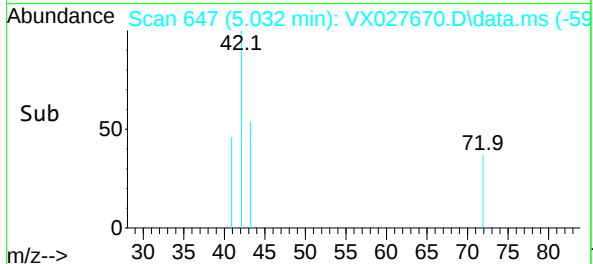

#31

Cyclohexane

Concen: 0.537 ug/l

RT: 5.464 min Scan# 718

Delta R.T. -0.006 min

Lab File: VX027670.D

Acq: 23 Mar 2022 16:14




Tgt Ion: 56 Resp: 2954


Ion Ratio Lower Upper

56 100

69 30.6 26.7 40.1

84 88.7 77.2 115.8

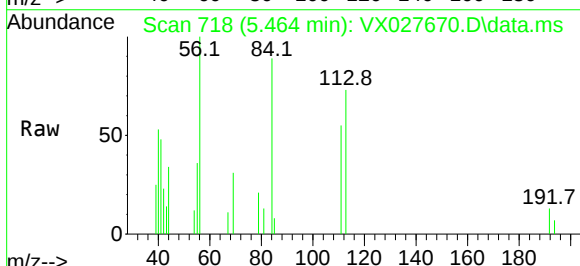



#33

1,2-Dichloroethane-d4

Concen: 44.255 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX027670.D

Acq: 23 Mar 2022 16:14

Instrument :

MSVOA_X

ClientSampleId :





WC-14A-2

Tgt Ion: 65 Resp: 195898

Ion Ratio Lower Upper

65 100

67 53.3 0.0 107.4

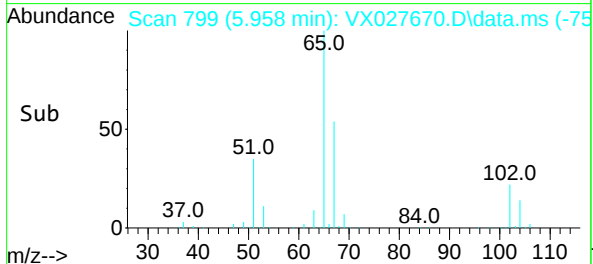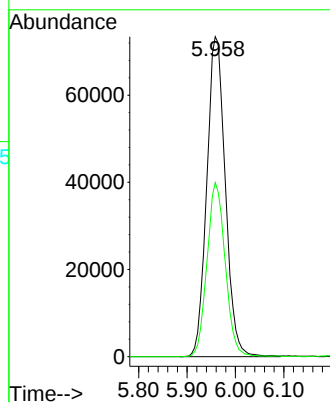

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.000 min

Lab File: VX027670.D

Acq: 23 Mar 2022 16:14




Tgt Ion: 114 Resp: 582104


Ion Ratio Lower Upper

114 100

63 18.2 0.0 36.8

88 15.9 0.0 32.4

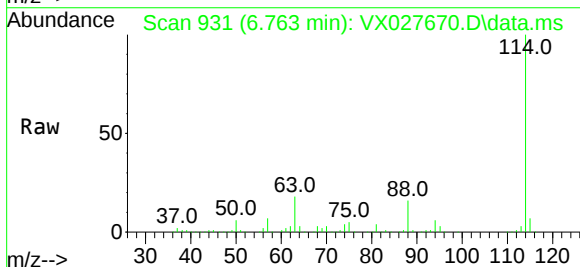



#35

Dibromofluoromethane

Concen: 49.871 ug/l

RT: 5.391 min Scan# 706

Delta R.T. 0.000 min

Lab File: VX027670.D

Acq: 23 Mar 2022 16:14

Instrument :

MSVOA_X

ClientSampleId :

WC-14A-2





Tgt Ion:113 Resp: 186776

Ion Ratio Lower Upper

113 100

111 101.1 82.8 124.2

192 20.5 16.9 25.3

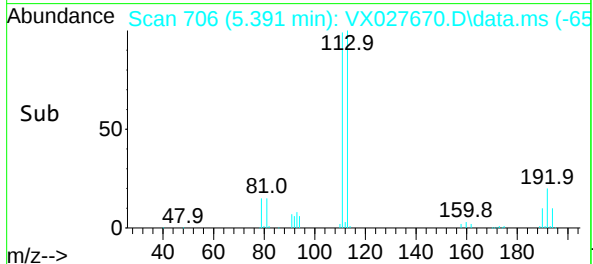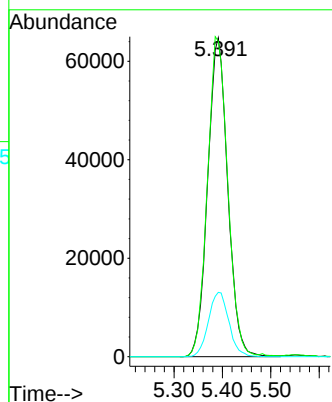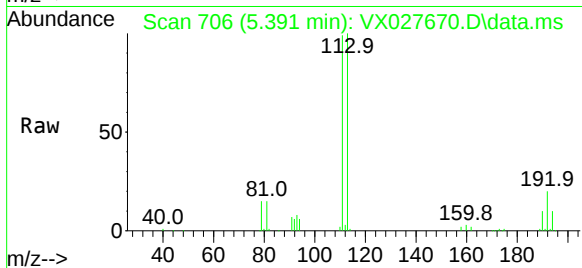

#36

1,1-Dichloropropene

Concen: 4.567 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.140 min

Lab File: VX027670.D

Acq: 23 Mar 2022 16:14




Tgt Ion: 75 Resp: 23375


Ion Ratio Lower Upper

75 100

110 9.8 18.3 54.8#

77 0.0 24.8 37.2#

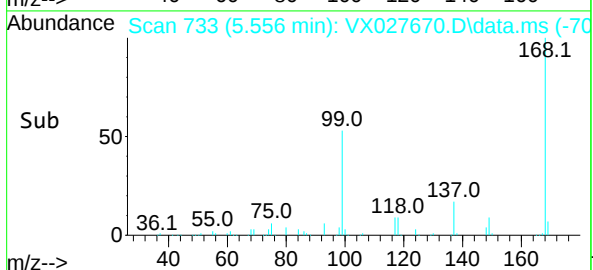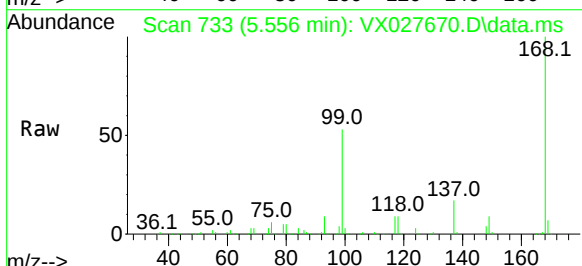



#37

Ethyl Acetate

Concen: 1.867 ug/l

RT: 4.568 min Scan# 51

Delta R.T. -0.152 min

Lab File: VX027670.D

Acq: 23 Mar 2022 16:14





Instrument :

MSVOA_X

ClientSampleId :

WC-14A-2

Tgt Ion:	43	Resp:	9522
Ion	Ratio	Lower	Upper
43	100		
61	0.2	12.6	19.0#
70	0.0	10.2	15.2#

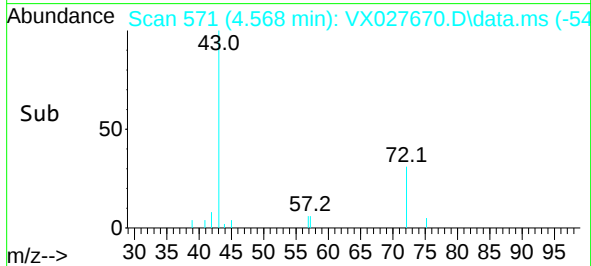

#38

Carbon Tetrachloride

Concen: 5.821 ug/l




RT: 5.550 min Scan# 732


Delta R.T. -0.128 min

Lab File: VX027670.D

Acq: 23 Mar 2022 16:14

Tgt Ion:	117	Resp:	34085
Ion	Ratio	Lower	Upper
117	100		
119	4.4	77.3	115.9#
121	0.0	24.2	36.2#

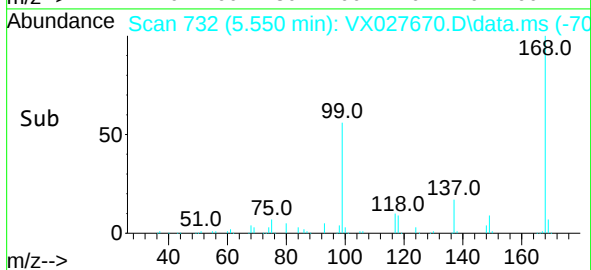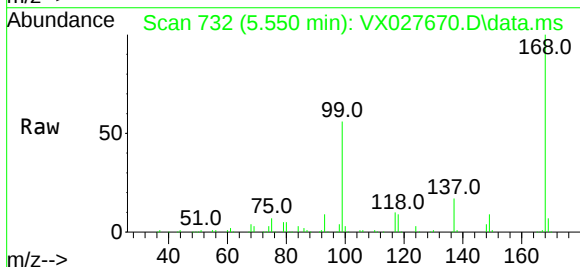



#39

Methylcyclohexane

Concen: 0.593 ug/l

RT: 7.385 min Scan# 1033

Delta R.T. 0.000 min

Lab File: VX027670.D

Acq: 23 Mar 2022 16:14

Instrument :

MSVOA_X

ClientSampleId :

WC-14A-2





Tgt Ion: 83 Resp: 3819

Ion Ratio Lower Upper

83 100

55 67.6 54.6 81.8

98 46.3 37.4 56.2

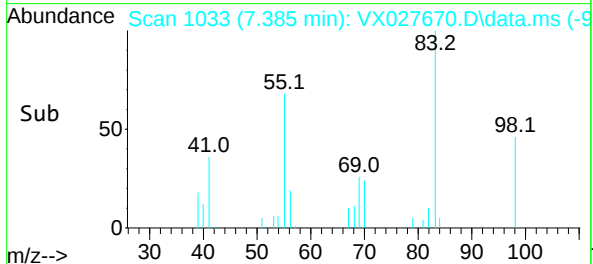

#43

Isopropyl Acetate

Concen: 3.157 ug/l

RT: 6.342 min Scan# 862

Delta R.T. 0.000 min

Lab File: VX027670.D

Acq: 23 Mar 2022 16:14




Tgt Ion: 43 Resp: 25911


Ion Ratio Lower Upper

43 100

61 21.8 18.5 27.7

87 15.5 13.0 19.6


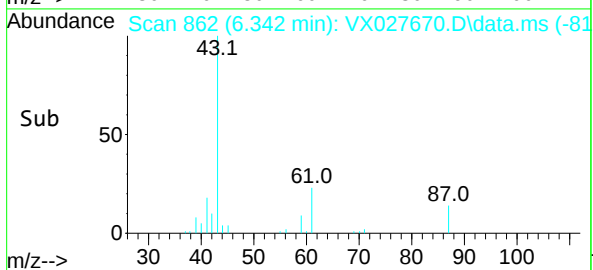

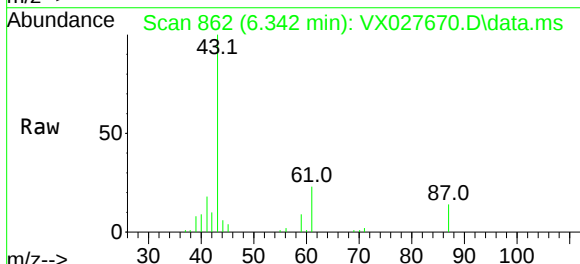




#48
Methyl methacrylate
Concen: 2.149 ug/l
RT: 7.598 min Scan# 1100
Delta R.T. -0.097 min
Lab File: VX027670.D
Acq: 23 Mar 2022 16:14




Instrument :
MSVOA_X
ClientSampleId :
WC-14A-2


Tgt Ion: 41 Resp: 8731
Ion Ratio Lower Upper
41 100
69 0.0 82.5 123.7#
39 0.0 43.8 65.8#

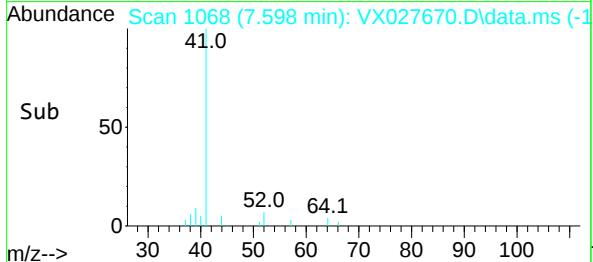

#49
1,4-Dioxane
Concen: 3.594 ug/l
RT: 7.793 min Scan# 1100
Delta R.T. 0.128 min
Lab File: VX027670.D
Acq: 23 Mar 2022 16:14

Tgt Ion: 88 Resp: 375
Ion Ratio Lower Upper
88 100
43 416434.9 21.9 32.9#
58 1850.9 53.7 80.5#


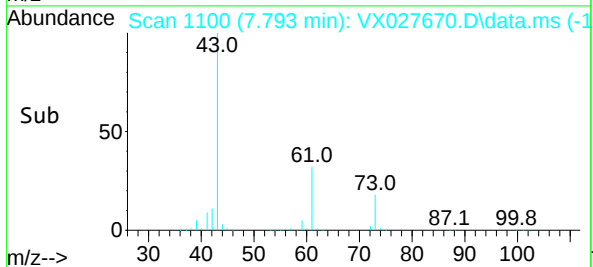

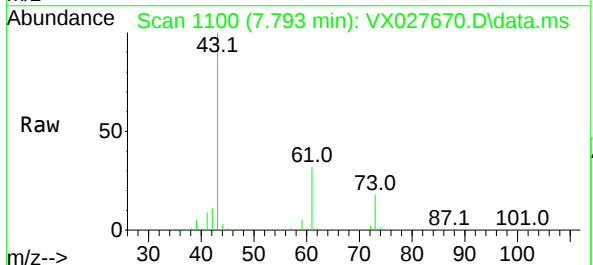




#50
Toluene-d8
Concen: 48.247 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.000 min
Lab File: VX027670.D
Acq: 23 Mar 2022 16:14




Instrument :
MSVOA_X
ClientSampleId :
WC-14A-2


Tgt Ion: 98 Resp: 683759
Ion Ratio Lower Upper
98 100
100 65.0 52.6 78.8

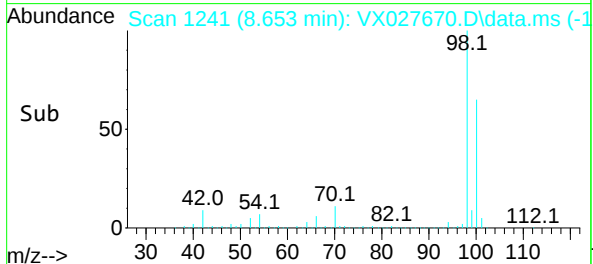

#51
4-Methyl-2-Pentanone
Concen: 14.612 ug/l
RT: 8.549 min Scan# 1224
Delta R.T. -0.030 min
Lab File: VX027670.D
Acq: 23 Mar 2022 16:14

Tgt Ion: 43 Resp: 76558
Ion Ratio Lower Upper
43 100
58 9.8 36.1 54.1#

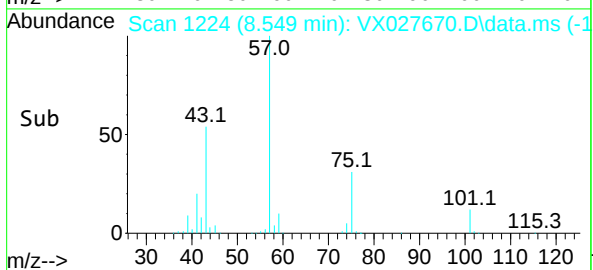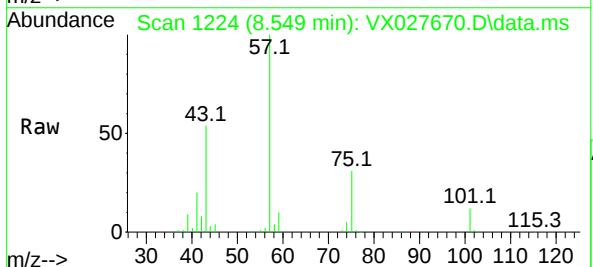



#52

Toluene

Concen: 0.219 ug/l

RT: 8.720 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX027670.D

Acq: 23 Mar 2022 16:14

Instrument :

MSVOA_X

ClientSampleId :





WC-14A-2

Tgt Ion: 92 Resp: 2155

Ion Ratio Lower Upper

92 100

91 199.1 137.5 206.3

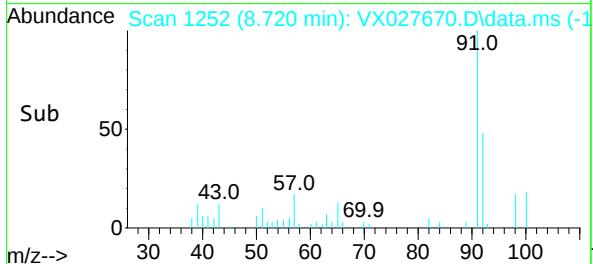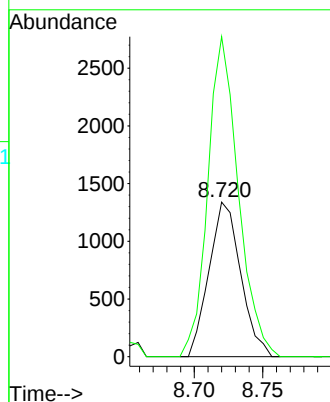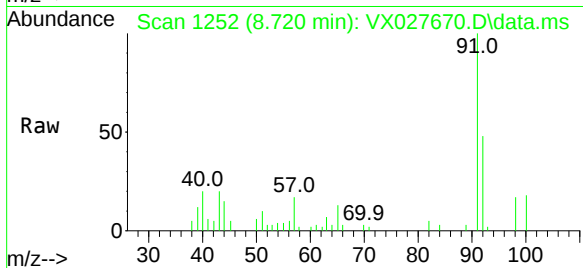

#54

cis-1,3-Dichloropropene

Concen: 6.566 ug/l

RT: 8.549 min Scan# 1224

Delta R.T. 0.177 min

Lab File: VX027670.D

Acq: 23 Mar 2022 16:14




Tgt Ion: 75 Resp: 39456


Ion Ratio Lower Upper

75 100

77 0.9 24.8 37.2#

39 28.3 29.6 44.4#

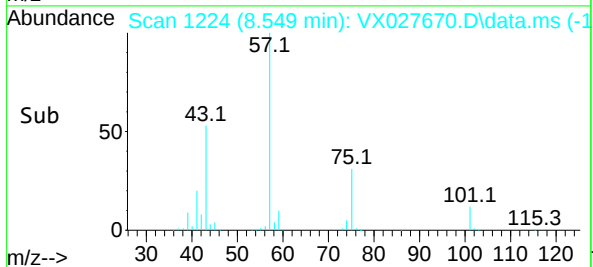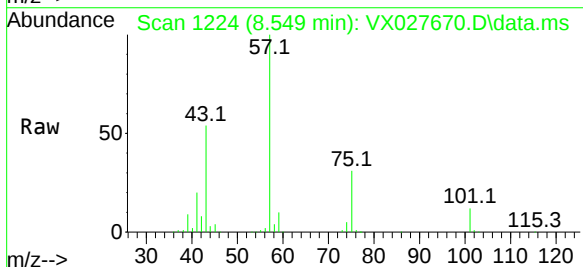



#57

1,3-Dichloropropane

Concen: 3.777 ug/l

RT: 9.482 min Scan# 1377

Delta R.T. 0.171 min

Lab File: VX027670.D

Acq: 23 Mar 2022 16:14

Instrument :

MSVOA_X

ClientSampleId :





WC-14A-2

Tgt Ion: 76 Resp: 24568

Ion Ratio Lower Upper

76 100

78 0.3 25.8 38.8#

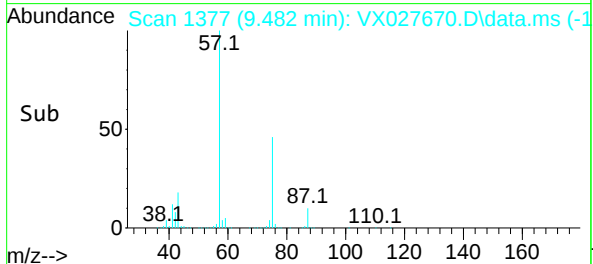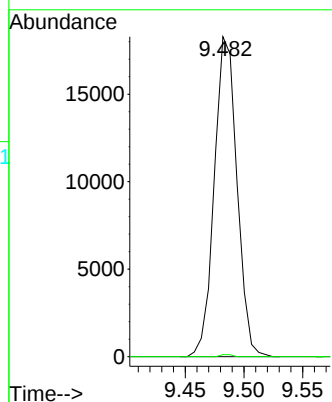

#59

2-Hexanone

Concen: 68.522 ug/l

RT: 9.482 min Scan# 1377

Delta R.T. 0.049 min

Lab File: VX027670.D




Acq: 23 Mar 2022 16:14


Tgt Ion: 43 Resp: 276506

Ion Ratio Lower Upper

43 100

58 21.1 31.9 95.7#

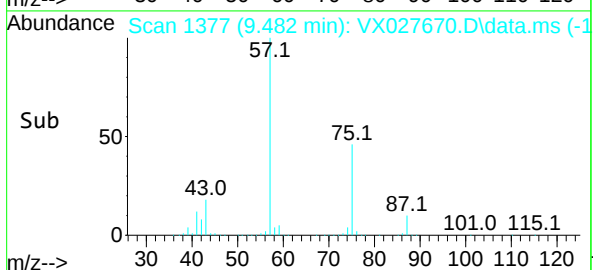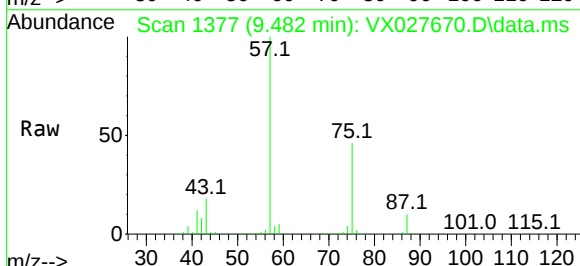

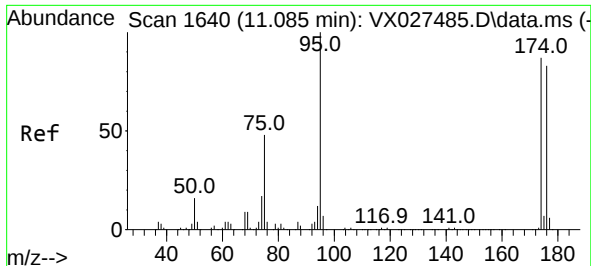

#62

4-Bromofluorobenzene

Concen: 54.185 ug/l

RT: 11.079 min Scan# 1

Delta R.T. -0.006 min

Lab File: VX027670.D

Acq: 23 Mar 2022 16:14

Instrument :

MSVOA_X

ClientSampleId :

WC-14A-2





Tgt Ion: 95 Resp: 282251

Ion Ratio Lower Upper

95 100

174 84.3 0.0 163.0

176 82.3 0.0 155.0

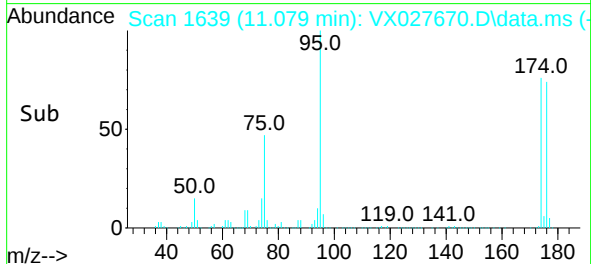

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX027670.D

Acq: 23 Mar 2022 16:14




Tgt Ion: 117 Resp: 549812


Ion Ratio Lower Upper

117 100

82 51.7 41.8 62.8

119 32.4 24.8 37.2

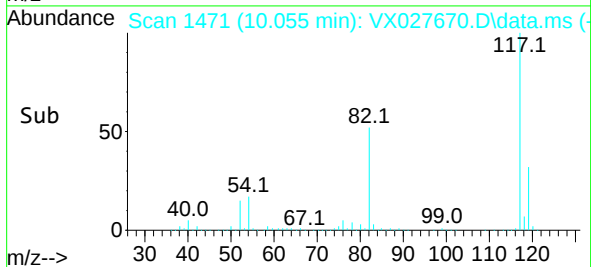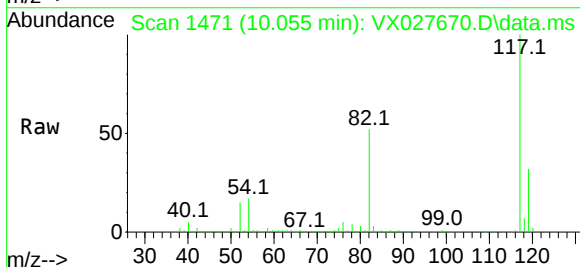

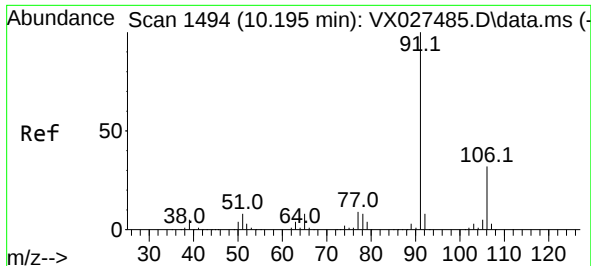

#67

Ethyl Benzene

Concen: 0.221 ug/l

RT: 10.195 min Scan# 1494

Delta R.T. 0.000 min

Lab File: VX027670.D

Acq: 23 Mar 2022 16:14

Instrument :

MSVOA_X

ClientSampleId :





WC-14A-2

Tgt Ion: 91 Resp: 4269

Ion Ratio Lower Upper

91 100

106 33.0 24.6 36.8

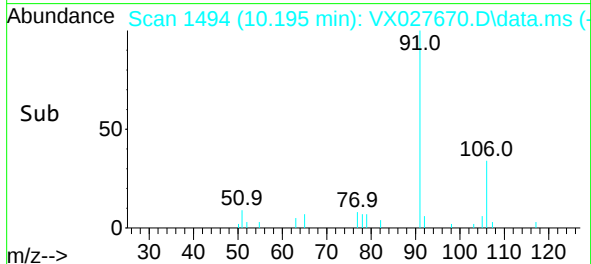

#68

m/p-Xylenes

Concen: 0.564 ug/l

RT: 10.305 min Scan# 1512

Delta R.T. 0.000 min

Lab File: VX027670.D




Acq: 23 Mar 2022 16:14


Tgt Ion: 106 Resp: 4298

Ion Ratio Lower Upper

106 100

91 190.3 160.4 240.6


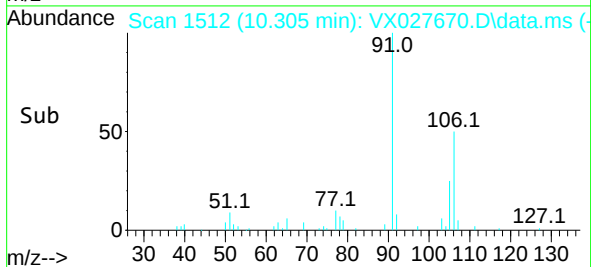

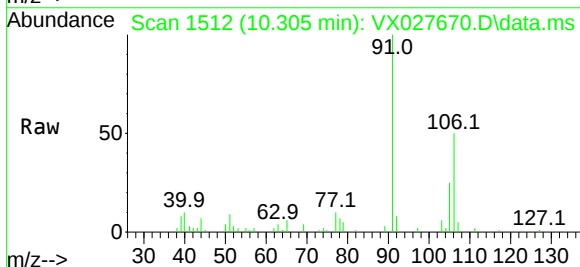




#69
o-Xylene
Concen: 1.520 ug/l
RT: 10.646 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX027670.D
Acq: 23 Mar 2022 16:14




Instrument :
MSVOA_X
ClientSampleId :
WC-14A-2


Tgt Ion:106 Resp: 11246
Ion Ratio Lower Upper
106 100
91 212.5 106.1 318.1

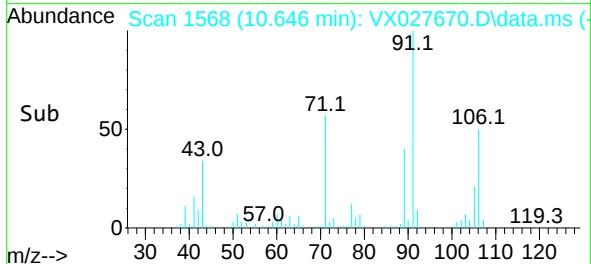

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX027670.D
Acq: 23 Mar 2022 16:14

Tgt Ion:152 Resp: 255572
Ion Ratio Lower Upper
152 100
115 58.5 37.5 112.7
150 156.6 0.0 338.2


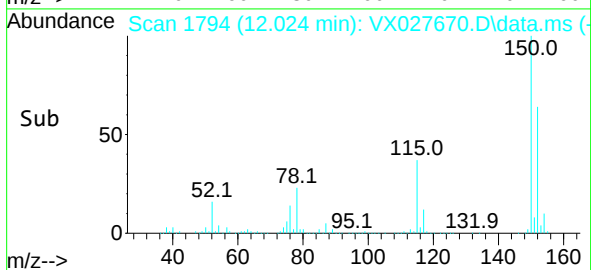

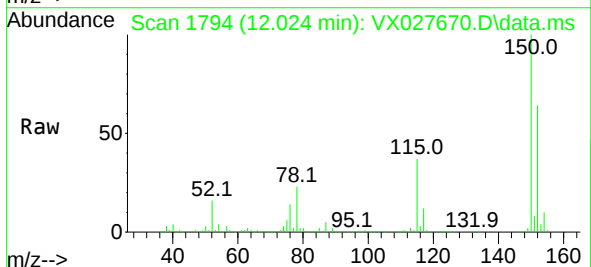




#76
1,2,3-Trichloropropane
Concen: 24.720 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.164 min
Lab File: VX027670.D
Acq: 23 Mar 2022 16:14




Instrument :
MSVOA_X
ClientSampleId :
WC-14A-2


Tgt Ion: 75 Resp: 132145
Ion Ratio Lower Upper
75 100
77 1.1 19.4 58.2#

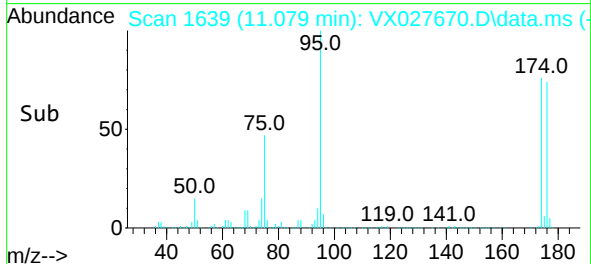

#80
1,3,5-Trimethylbenzene
Concen: 0.798 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. 0.000 min
Lab File: VX027670.D
Acq: 23 Mar 2022 16:14

Tgt Ion:105 Resp: 12510
Ion Ratio Lower Upper
105 100
120 48.3 24.3 72.9



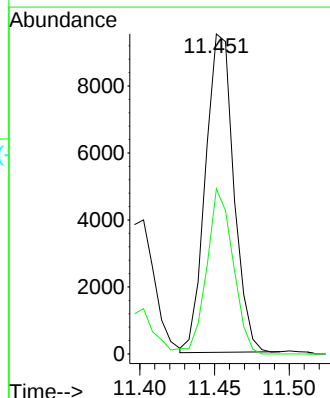
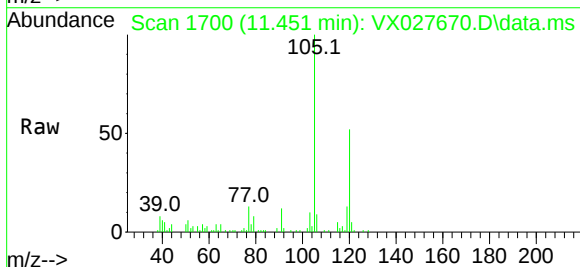


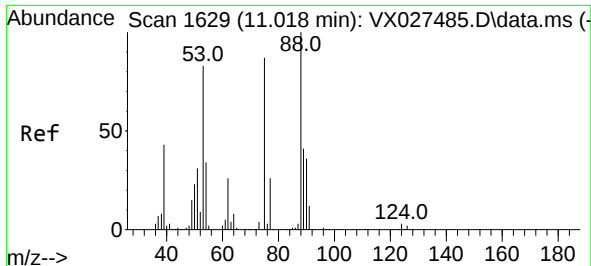

#81
trans-1,4-Dichloro-2-butene
Concen: 75.075 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX027670.D
Acq: 23 Mar 2022 16:14




Instrument :
MSVOA_X
ClientSampleId :
WC-14A-2


Tgt Ion: 75 Resp: 132145
Ion Ratio Lower Upper
75 100
53 0.0 69.0 103.4#
89 0.0 37.0 55.6#

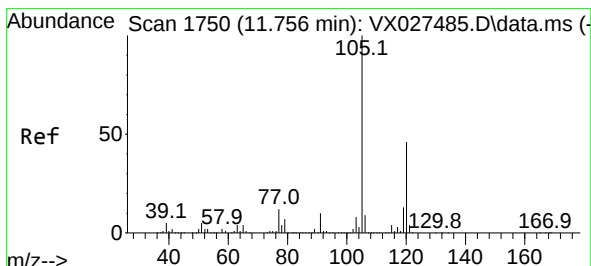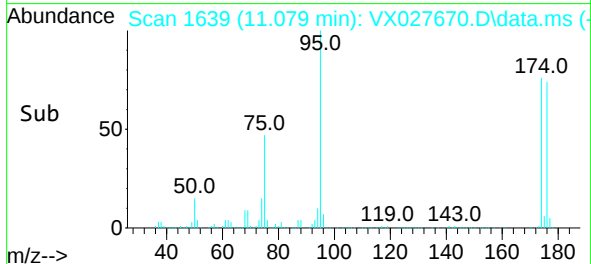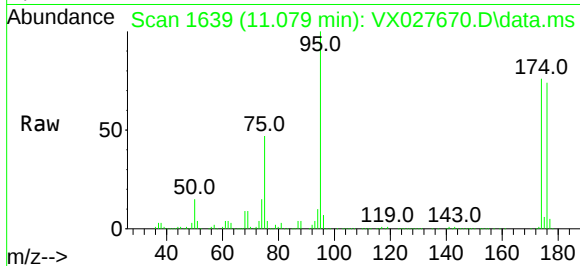

#84
1,2,4-Trimethylbenzene
Concen: 1.918 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.000 min
Lab File: VX027670.D
Acq: 23 Mar 2022 16:14

Tgt Ion: 105 Resp: 29968
Ion Ratio Lower Upper
105 100
120 44.1 22.6 67.8


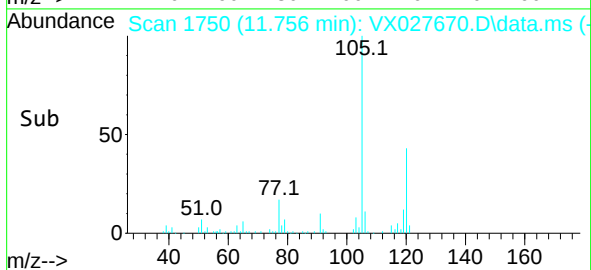

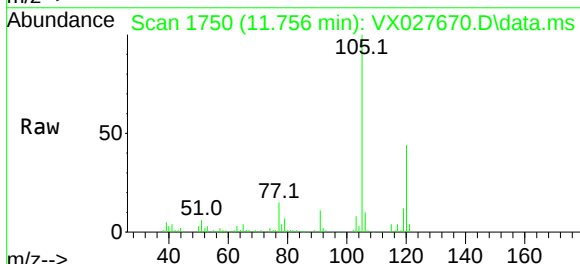




#89
n-Butylbenzene
Concen: 0.202 ug/l
RT: 12.323 min Scan# 1845
Delta R.T. -0.012 min
Lab File: VX027670.D
Acq: 23 Mar 2022 16:14

Instrument :
MSVOA_X
ClientSampleId :
WC-14A-2

Tgt Ion: 91 Resp: 2722
Ion Ratio Lower Upper
91 100
92 24.3 27.8 83.3#
134 108.8 13.3 39.8#

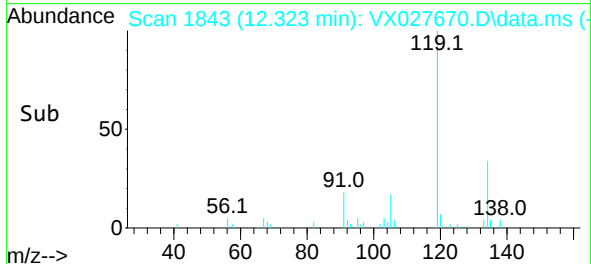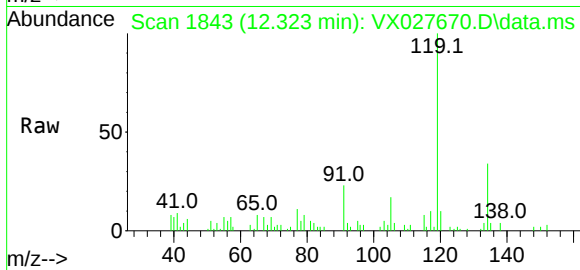

#95
Naphthalene
Concen: 2.553 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.000 min
Lab File: VX027670.D
Acq: 23 Mar 2022 16:14

Tgt Ion: 128 Resp: 45221
Ion Ratio Lower Upper
128 100
127 12.9 10.2 15.4
129 12.7 8.7 13.1

