

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032322\
 Data File : VX027658.D
 Acq On : 23 Mar 2022 11:05
 Operator : JC/MD
 Sample : VX0323WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0323WBL01

Quant Time: Mar 23 17:25:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 17 15:02:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	360816	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	584793	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	518703	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	244706	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	211815	47.654	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	95.300%
35) Dibromofluoromethane	5.391	113	190492	50.630	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	101.260%
50) Toluene-d8	8.653	98	679962	47.758	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	95.520%
62) 4-Bromofluorobenzene	11.079	95	245363	46.887	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	93.780%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032322\
Data File : VX027658.D
Acq On : 23 Mar 2022 11:05
Operator : JC/MD
Sample : VX0323WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0323WBL01

Quant Time: Mar 23 17:25:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260
QLast Update : Thu Mar 17 15:02:59 2022
Response via : Initial Calibration




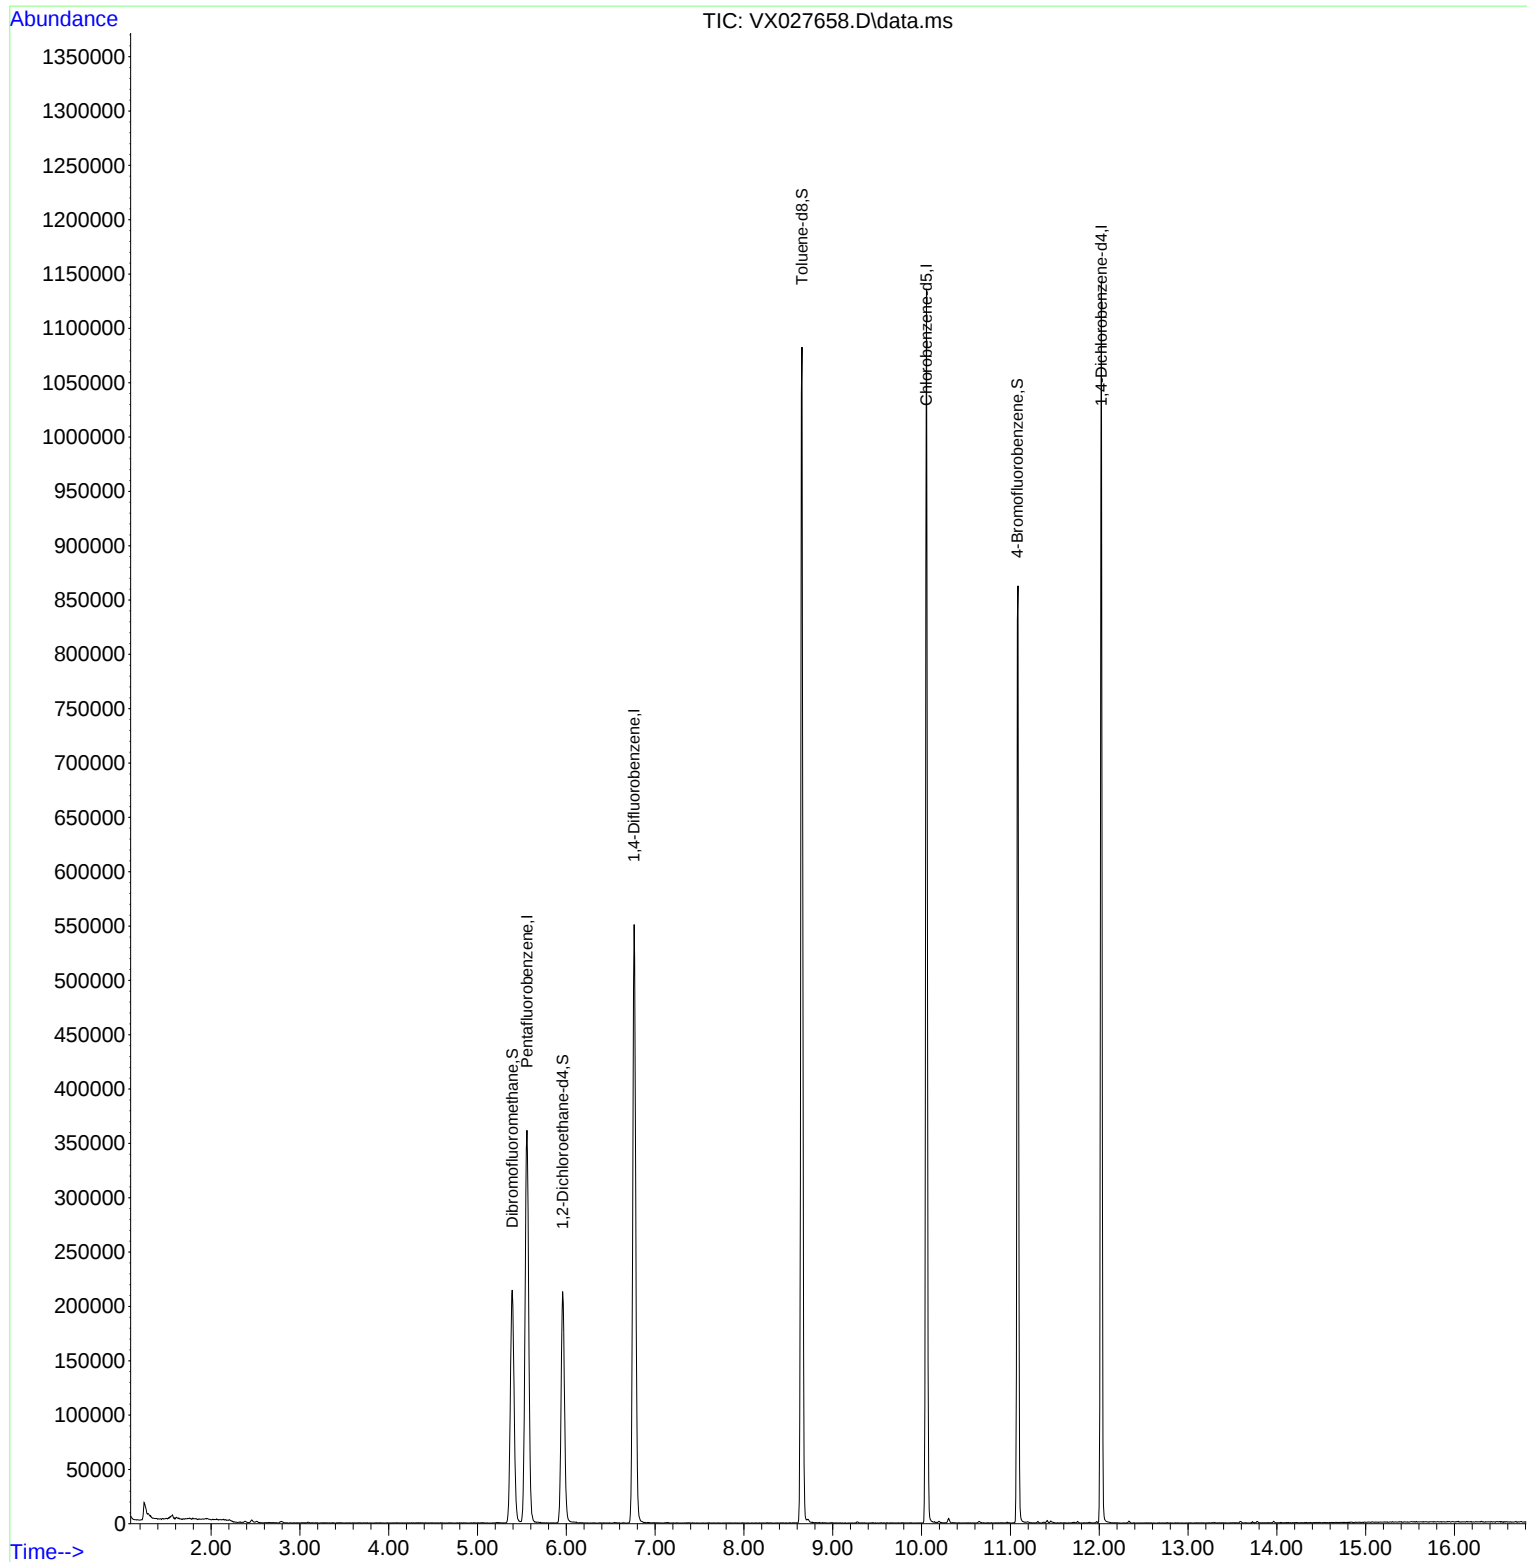




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 713
Delta R.T. -0.000 min
Lab File: VX027658.D
Acq: 23 Mar 2022 11:05




Instrument :
MSVOA_X
ClientSampleId :
VX0323WBL01


Tgt Ion:168 Resp: 360816
Ion Ratio Lower Upper
168 100
99 54.2 41.7 62.5

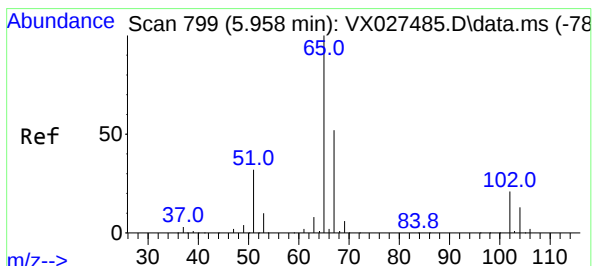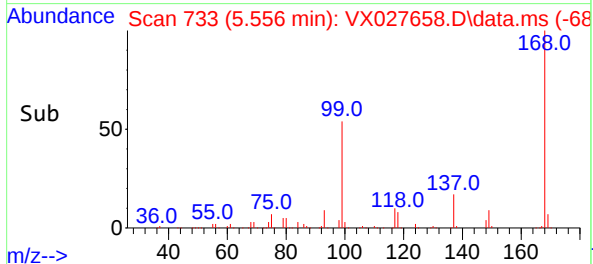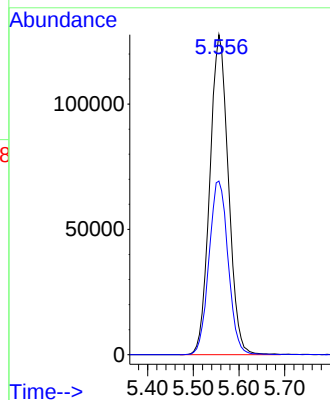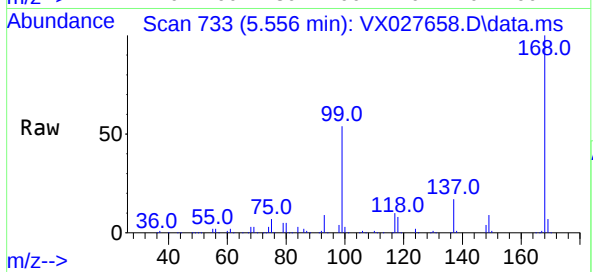

#33
1,2-Dichloroethane-d4
Concen: 47.654 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX027658.D
Acq: 23 Mar 2022 11:05

Tgt Ion: 65 Resp: 211815
Ion Ratio Lower Upper
65 100
67 52.0 0.0 107.4


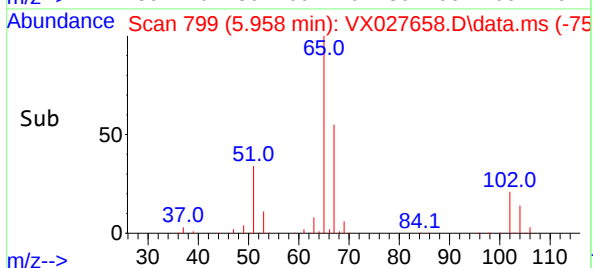
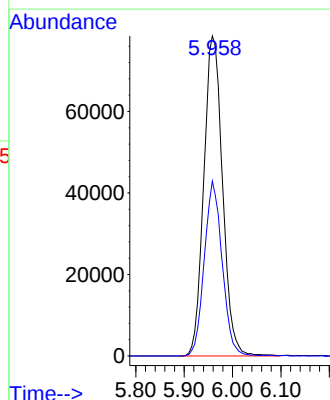
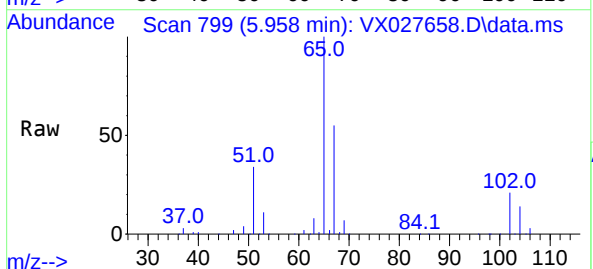


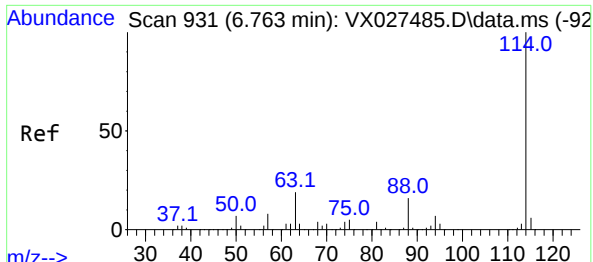

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX027658.D
Acq: 23 Mar 2022 11:05




Instrument :
MSVOA_X
ClientSampleId :
VX0323WBL01


Tgt Ion:114 Resp: 584793
Ion Ratio Lower Upper
114 100
63 17.9 0.0 36.8
88 16.0 0.0 32.4

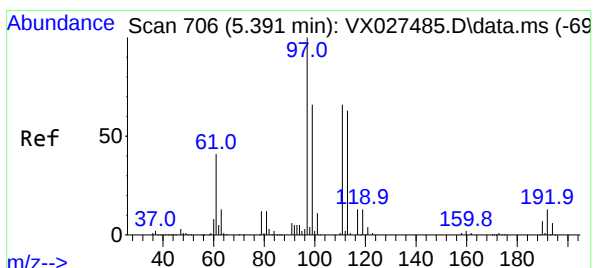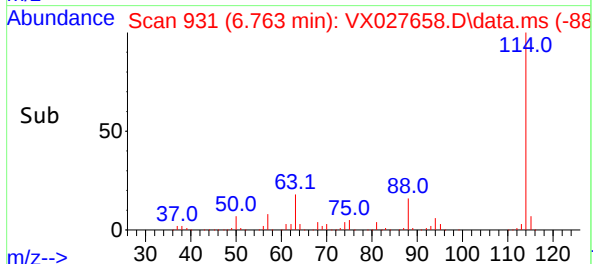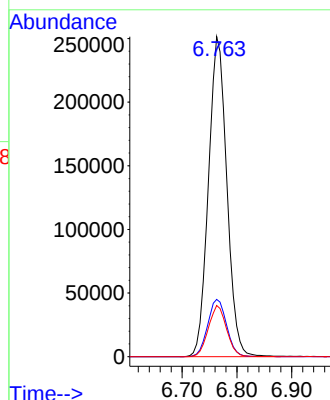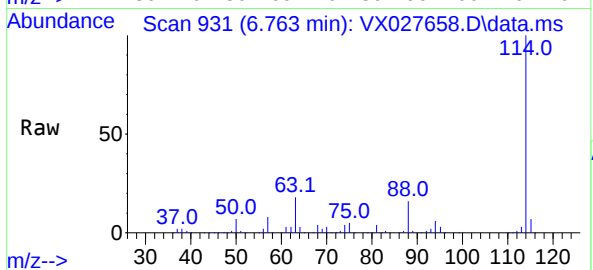

#35
Dibromofluoromethane
Concen: 50.630 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX027658.D
Acq: 23 Mar 2022 11:05

Tgt Ion:113 Resp: 190492
Ion Ratio Lower Upper
113 100
111 102.8 82.8 124.2
192 20.5 16.9 25.3


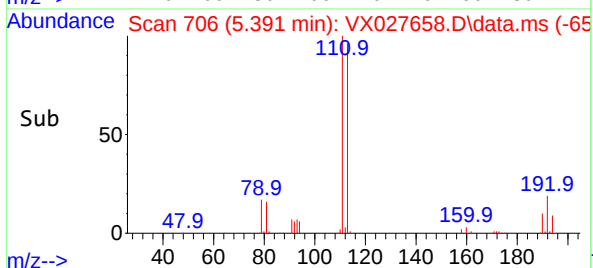
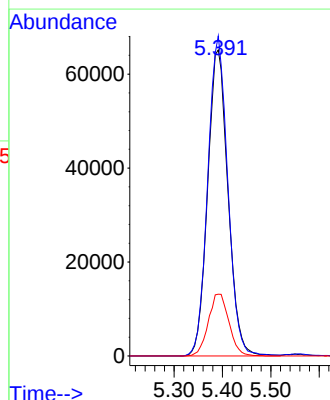
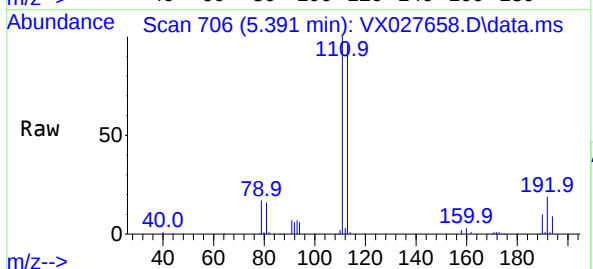


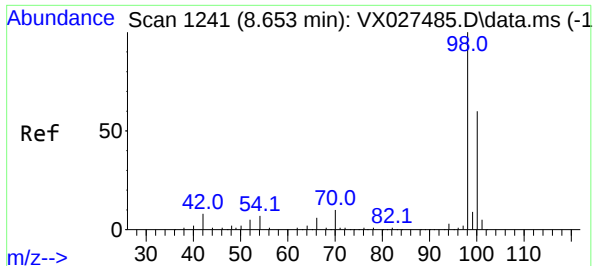

#50
Toluene-d8
Concen: 47.758 ug/l
RT: 8.653 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX027658.D
Acq: 23 Mar 2022 11:05




Instrument :
MSVOA_X
ClientSampleId :
VX0323WBL01


Tgt Ion: 98 Resp: 679962
Ion Ratio Lower Upper
98 100
100 64.7 52.6 78.8

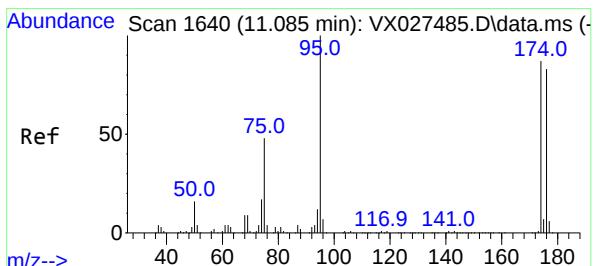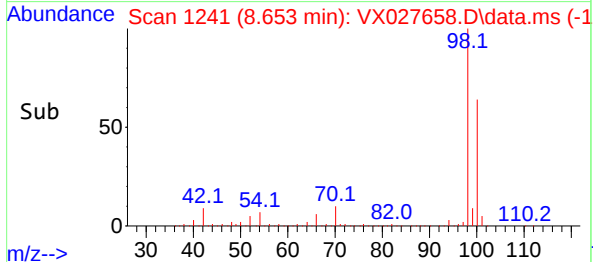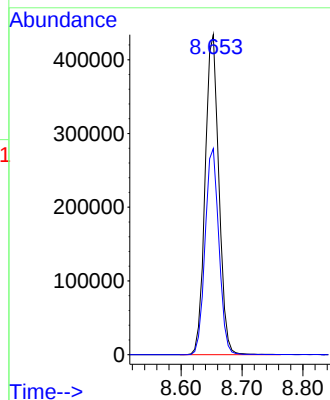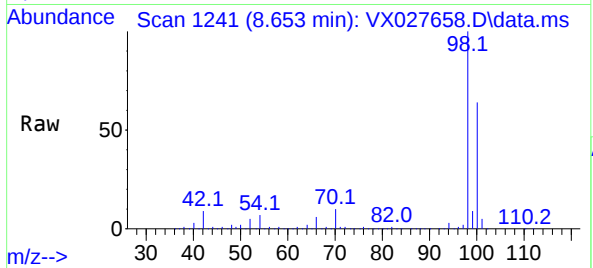

#62
4-Bromofluorobenzene
Concen: 46.887 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.006 min
Lab File: VX027658.D
Acq: 23 Mar 2022 11:05

Tgt Ion: 95 Resp: 245363
Ion Ratio Lower Upper
95 100
174 85.2 0.0 163.0
176 81.2 0.0 155.0


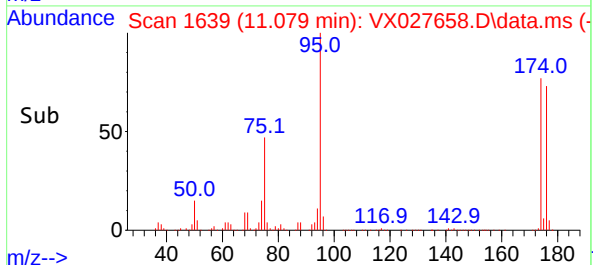
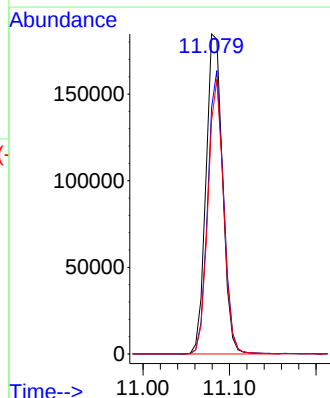
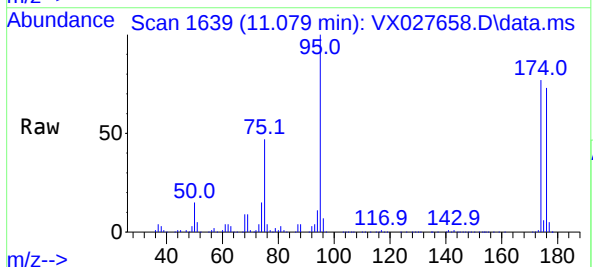


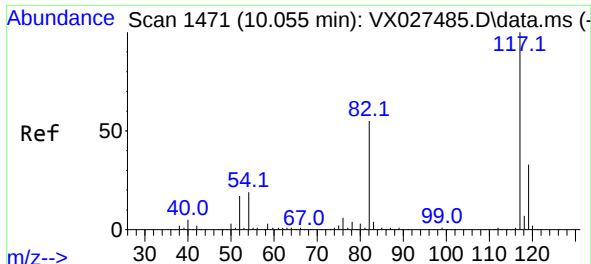

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX027658.D
Acq: 23 Mar 2022 11:05

Instrument :
MSVOA_X
ClientSampleId :
VX0323WBL01

Tgt Ion:117 Resp: 518703
Ion Ratio Lower Upper
117 100
82 54.0 41.8 62.8
119 33.0 24.8 37.2

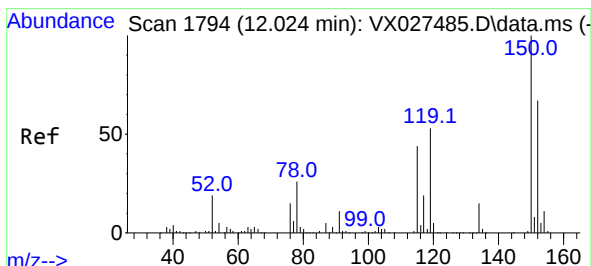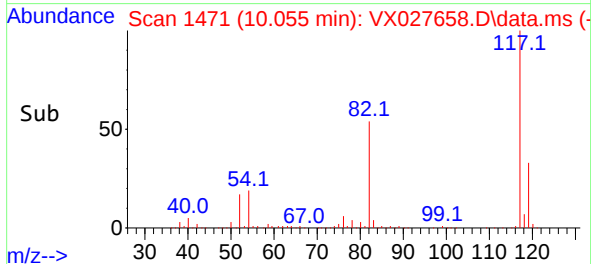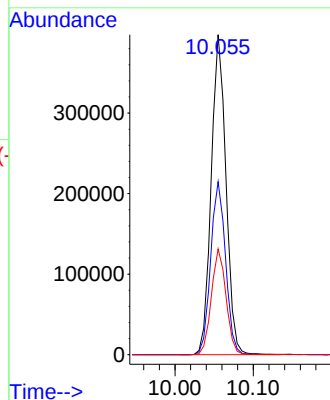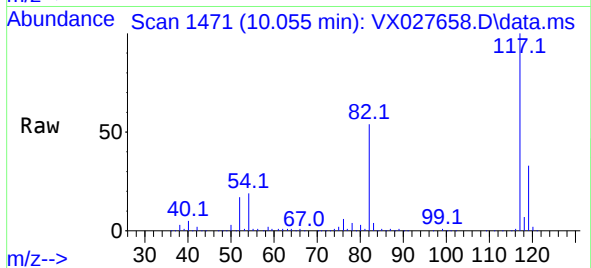

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX027658.D
Acq: 23 Mar 2022 11:05

Tgt Ion:152 Resp: 244706
Ion Ratio Lower Upper
152 100
115 59.0 37.5 112.7
150 155.9 0.0 338.2

