

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032322\
 Data File : VX027661.D
 Acq On : 23 Mar 2022 12:42
 Operator : JC/MD
 Sample : N1998-19DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP031622DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
 Title : SW846 8260

Signal : TIC: VX027661.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.111	321	332	342	rVB4	18158	49018	1.10%	0.189%
2	4.306	520	528	539	rVB3	28367	78098	1.75%	0.301%
3	5.391	694	706	716	rBV	203285	601507	13.50%	2.317%
4	5.556	724	733	761	rVB	352956	1032311	23.17%	3.977%
5	5.964	789	800	807	rBV	200433	523048	11.74%	2.015%
6	6.043	807	813	826	rVB2	54798	151484	3.40%	0.584%
7	6.251	839	847	856	rVB5	13850	49067	1.10%	0.189%
8	6.769	921	932	942	rBV	510950	1220206	27.39%	4.701%
9	7.379	1021	1032	1043	rBV4	37029	96846	2.17%	0.373%
10	8.653	1234	1241	1247	rBV	1051400	1625989	36.50%	6.264%
11	8.720	1247	1252	1259	rVB	449934	682352	15.32%	2.629%
12	10.055	1460	1471	1477	rBV	1086300	1469391	32.98%	5.661%
13	10.195	1489	1494	1501	rBV	1707249	2166575	48.63%	8.346%
14	10.305	1505	1512	1523	rVB	3196174	4455370	100.00%	17.164%
15	10.640	1562	1567	1583	rVB	943158	1273080	28.57%	4.904%
16	10.963	1613	1620	1625	rVB	46325	58301	1.31%	0.225%
17	11.085	1634	1640	1645	rBV	841998	1115132	25.03%	4.296%
18	11.305	1672	1676	1681	rVB	172268	209221	4.70%	0.806%
19	11.378	1681	1688	1696	rVV	634840	1164092	26.13%	4.484%
20	11.451	1696	1700	1712	rVB	797711	975915	21.90%	3.760%
21	11.616	1721	1727	1735	rVB	372048	472074	10.60%	1.819%
22	11.713	1735	1743	1745	rBV	49007	68828	1.54%	0.265%
23	11.756	1745	1750	1755	rVB	1425661	1810431	40.63%	6.974%
24	11.890	1764	1772	1778	rVB6	31635	63774	1.43%	0.246%
25	12.024	1789	1794	1800	rBV	1043876	1275476	28.63%	4.914%
26	12.091	1800	1805	1812	rBV	606032	766341	17.20%	2.952%
27	12.244	1823	1830	1838	rBV3	309884	469400	10.54%	1.808%
28	12.323	1838	1843	1852	rVB2	189413	271801	6.10%	1.047%
29	12.463	1862	1866	1871	rBV	37924	49652	1.11%	0.191%
30	12.530	1871	1877	1879	rBV	81566	104250	2.34%	0.402%
31	12.555	1879	1881	1886	rVV	78383	91921	2.06%	0.354%
32	12.615	1886	1891	1894	rVV	177471	203249	4.56%	0.783%
33	12.701	1900	1905	1911	rVB2	58488	93536	2.10%	0.360%
34	12.847	1925	1929	1935	rVB2	50584	71414	1.60%	0.275%
35	12.920	1935	1941	1945	rVV	110489	136998	3.07%	0.528%
36	12.963	1945	1948	1954	rVB	186614	214683	4.82%	0.827%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032322\
Data File : VX027661.D
Acq On : 23 Mar 2022 12:42
Operator : JC/MD
Sample : N1998-19DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP031622DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M

Title : SW846 8260

37	13.170	1978	1982	1986	rVB	42570	49473	1.11%	0.191%
38	13.292	1998	2002	2007	rVB2	116200	155068	3.48%	0.597%
39	13.347	2007	2011	2020	rVB	46768	73725	1.65%	0.284%
40	13.713	2067	2071	2076	rVB	59267	78245	1.76%	0.301%
41	13.774	2076	2081	2087	rVB	299428	385802	8.66%	1.486%
42	13.871	2093	2097	2103	rVB	40843	55077	1.24%	0.212%




Sum of corrected areas: 25958221

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032322\
Data File : VX027661.D
Acq On : 23 Mar 2022 12:42
Operator : JC/MD
Sample : N1998-19DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP031622DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

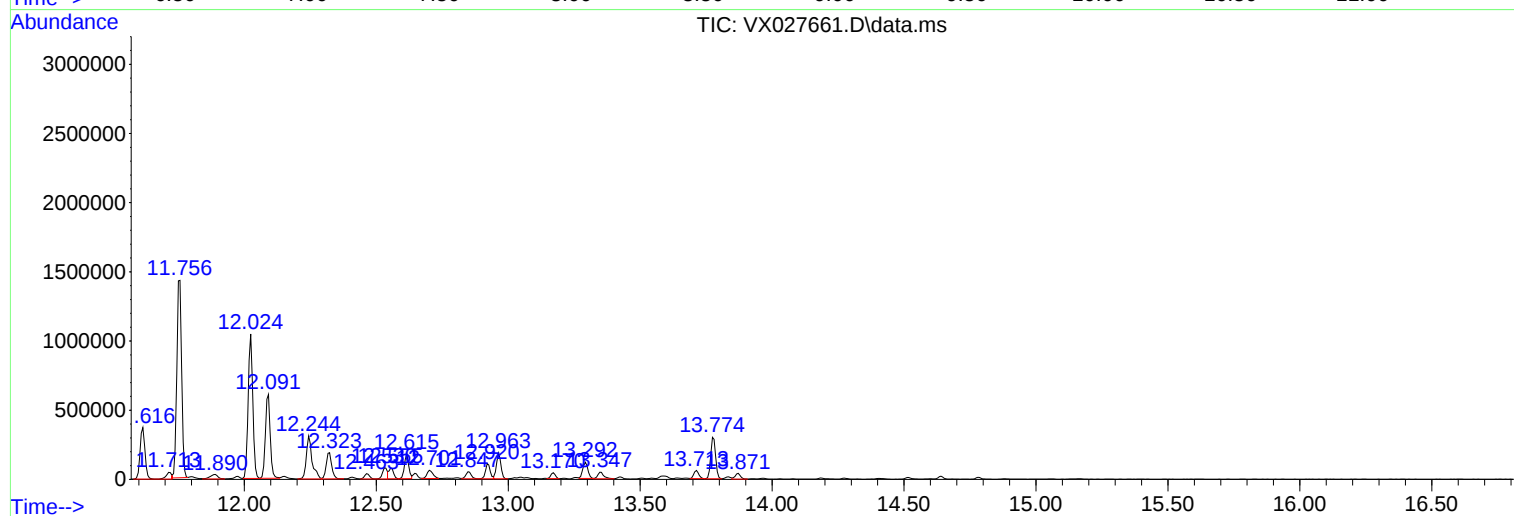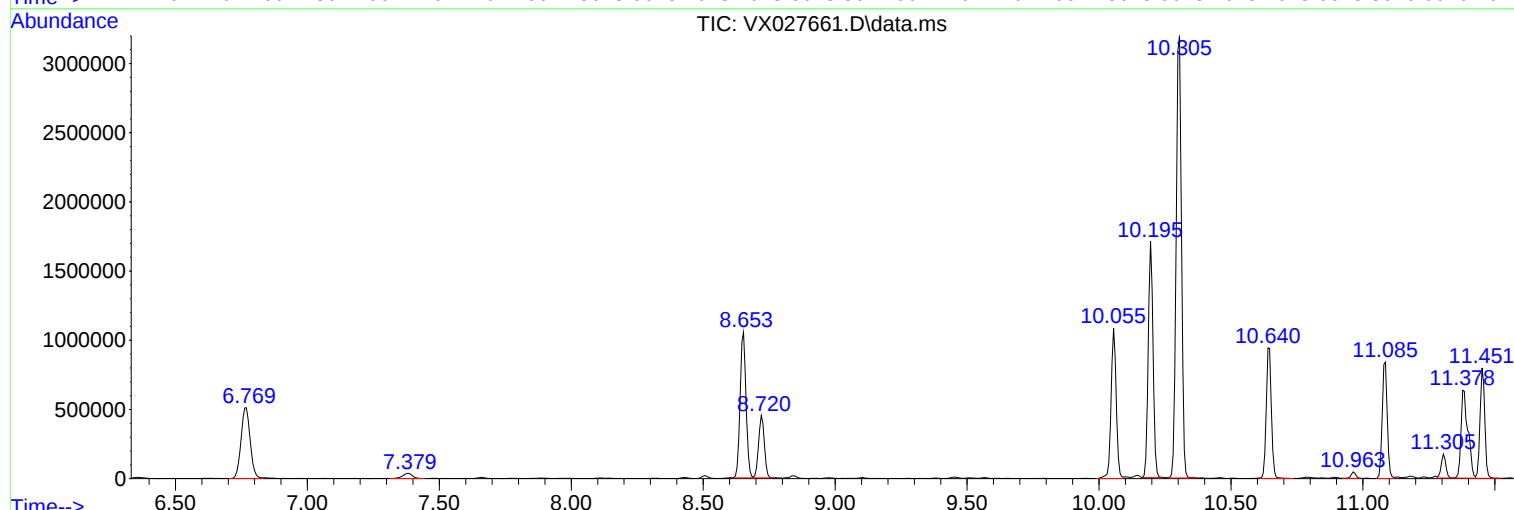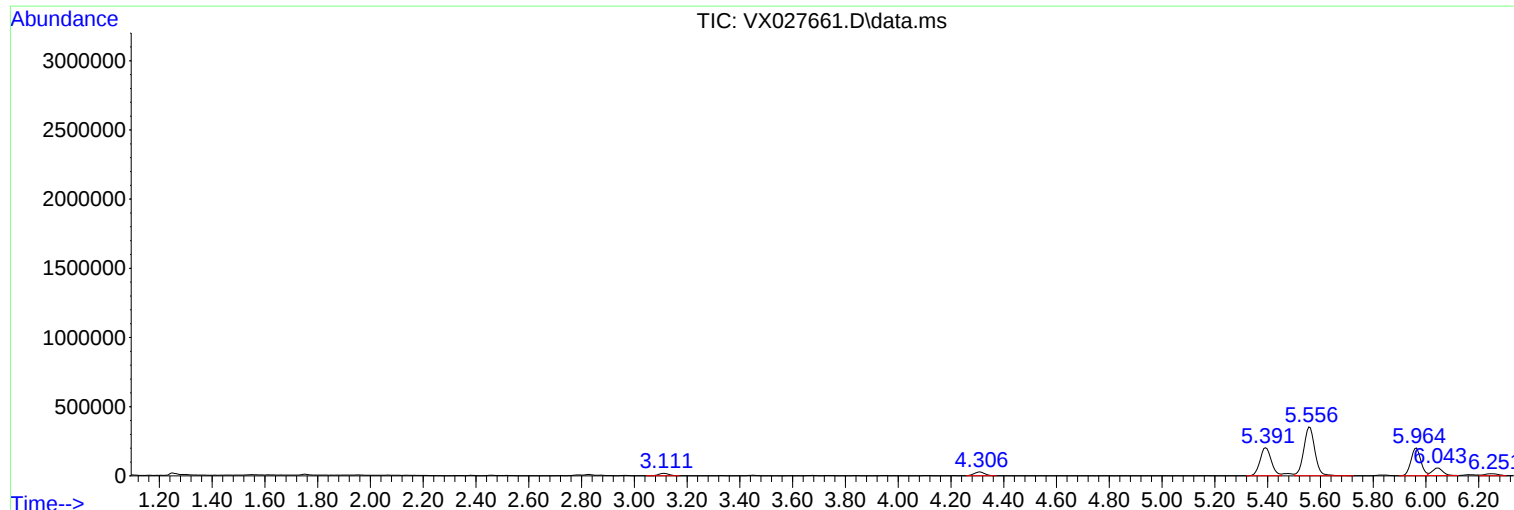

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032322\
Data File : VX027661.D
Acq On : 23 Mar 2022 12:42
Operator : JC/MD
Sample : N1998-19DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP031622DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032322\
Data File : VX027661.D
Acq On : 23 Mar 2022 12:42
Operator : JC/MD
Sample : N1998-19DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP031622DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc