

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032322\
 Data File : VX027662.D
 Acq On : 23 Mar 2022 13:05
 Operator : JC/MD
 Sample : N1998-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FB031522

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M

Title : SW846 8260

Signal : TIC: VX027662.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	32	rBV	19902	36882	2.24%	0.408%
2	2.538	231	238	246	rVB	9140	17193	1.04%	0.190%
3	2.946	297	305	317	rBV2	10586	24064	1.46%	0.266%
4	5.391	693	706	721	rBV	196240	572867	34.72%	6.340%
5	5.556	721	733	750	rVB	362138	1017457	61.66%	11.260%
6	5.958	789	799	816	rBV	205704	537032	32.55%	5.943%
7	6.763	922	931	947	rBV	526461	1242935	75.32%	13.755%
8	8.653	1234	1241	1251	rBV	1060284	1650101	100.00%	18.261%
9	10.055	1465	1471	1483	rBV	1088768	1455613	88.21%	16.109%
10	11.085	1634	1640	1654	rBV	849272	1121696	67.98%	12.413%
11	12.024	1788	1794	1811	rBV	1108587	1360324	82.44%	15.054%




Sum of corrected areas: 9036164

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032322\
Data File : VX027662.D
Acq On : 23 Mar 2022 13:05
Operator : JC/MD
Sample : N1998-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB031522

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

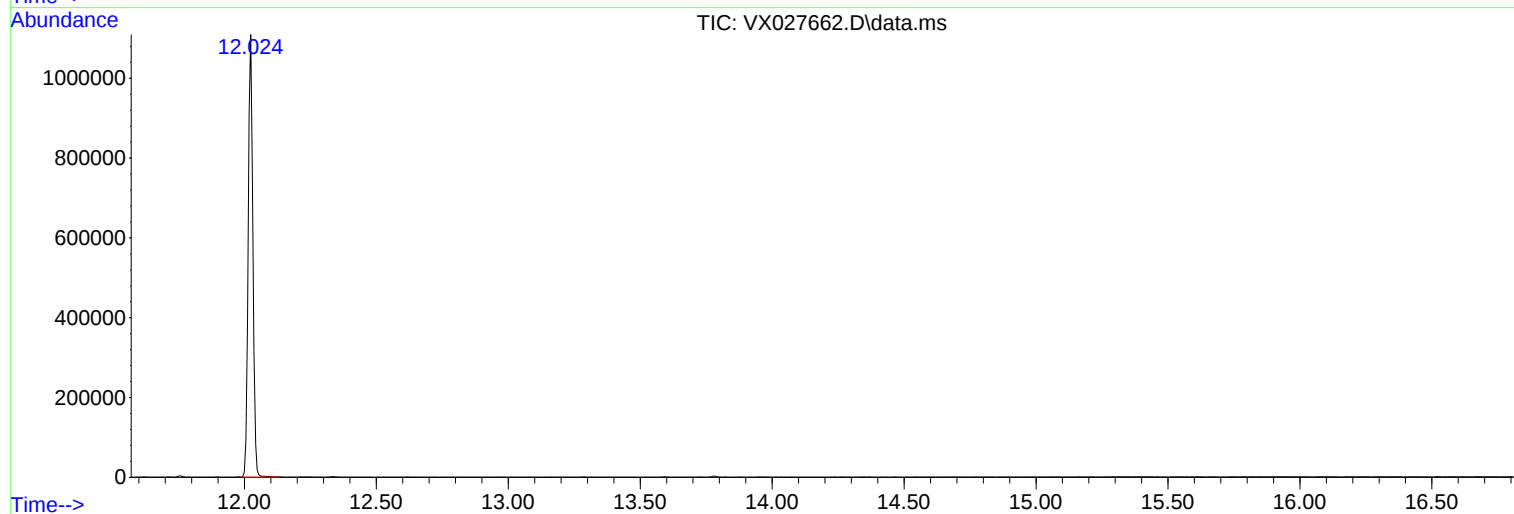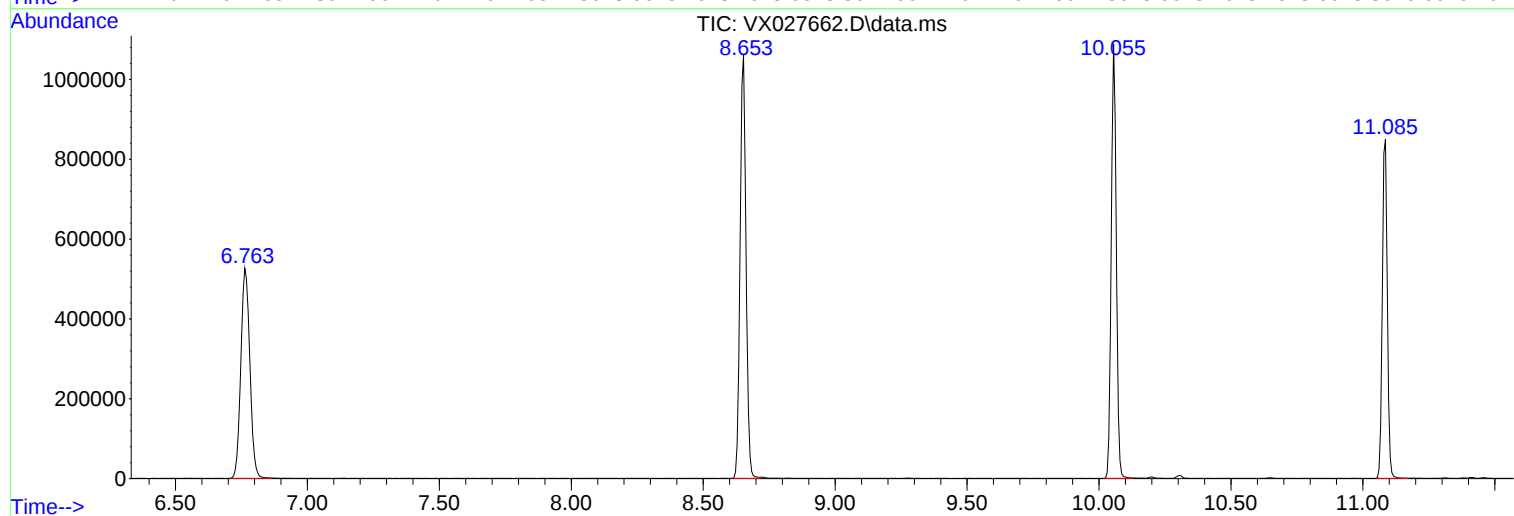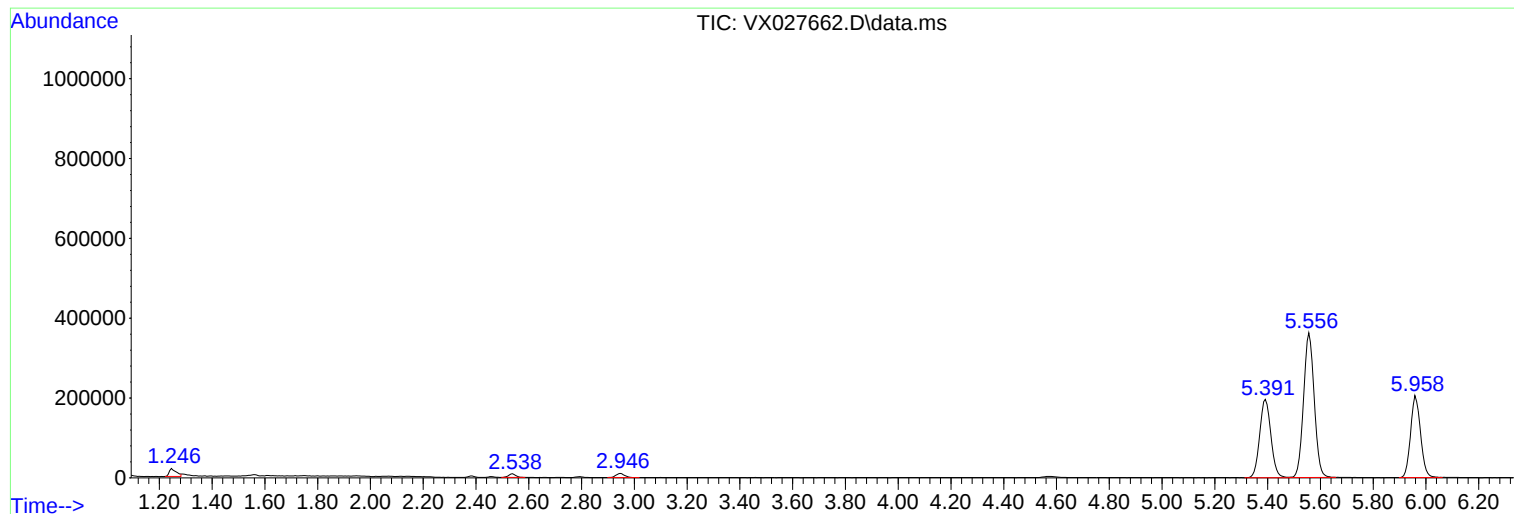

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032322\
Data File : VX027662.D
Acq On : 23 Mar 2022 13:05
Operator : JC/MD
Sample : N1998-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB031522

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032322\
Data File : VX027662.D
Acq On : 23 Mar 2022 13:05
Operator : JC/MD
Sample : N1998-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB031522

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc