

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032322\
 Data File : VX027665.D
 Acq On : 23 Mar 2022 14:16
 Operator : JC/MD
 Sample : N2028-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-116D

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
 Title : SW846 8260

Signal : TIC: VX027665.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	43	rBV	17645	45354	2.82%	0.519%
2	2.538	230	238	248	rBV	20035	39647	2.47%	0.454%
3	2.947	297	305	314	rBV	8098	19149	1.19%	0.219%
4	5.391	692	706	721	rBV	198647	575214	35.80%	6.588%
5	5.556	721	733	750	rVB	338390	950511	59.16%	10.887%
6	5.958	789	799	812	rBV	197507	523437	32.58%	5.995%
7	6.763	920	931	949	rBV	500725	1192292	74.21%	13.656%
8	8.653	1234	1241	1257	rBV	1025604	1606583	100.00%	18.402%
9	10.055	1465	1471	1488	rBV	1067756	1419183	88.34%	16.255%
10	11.085	1634	1640	1653	rBV	812818	1079562	67.20%	12.365%
11	12.024	1788	1794	1803	rBV	1023501	1279774	79.66%	14.658%




Sum of corrected areas: 8730706

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032322\
Data File : VX027665.D
Acq On : 23 Mar 2022 14:16
Operator : JC/MD
Sample : N2028-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-116D

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

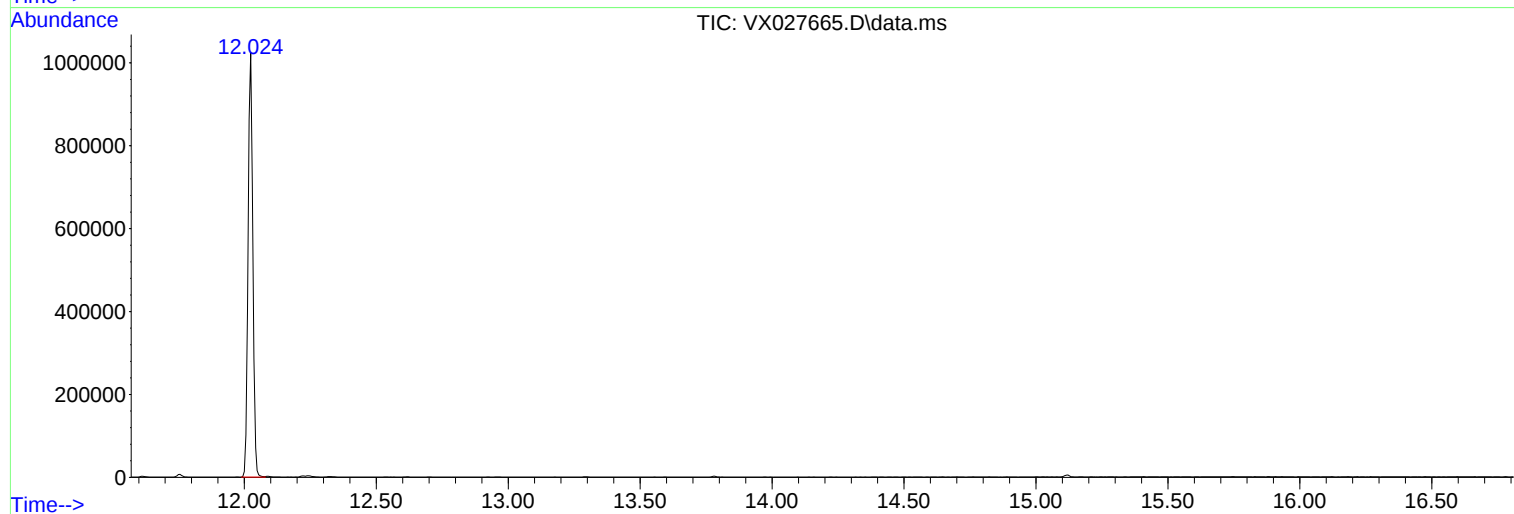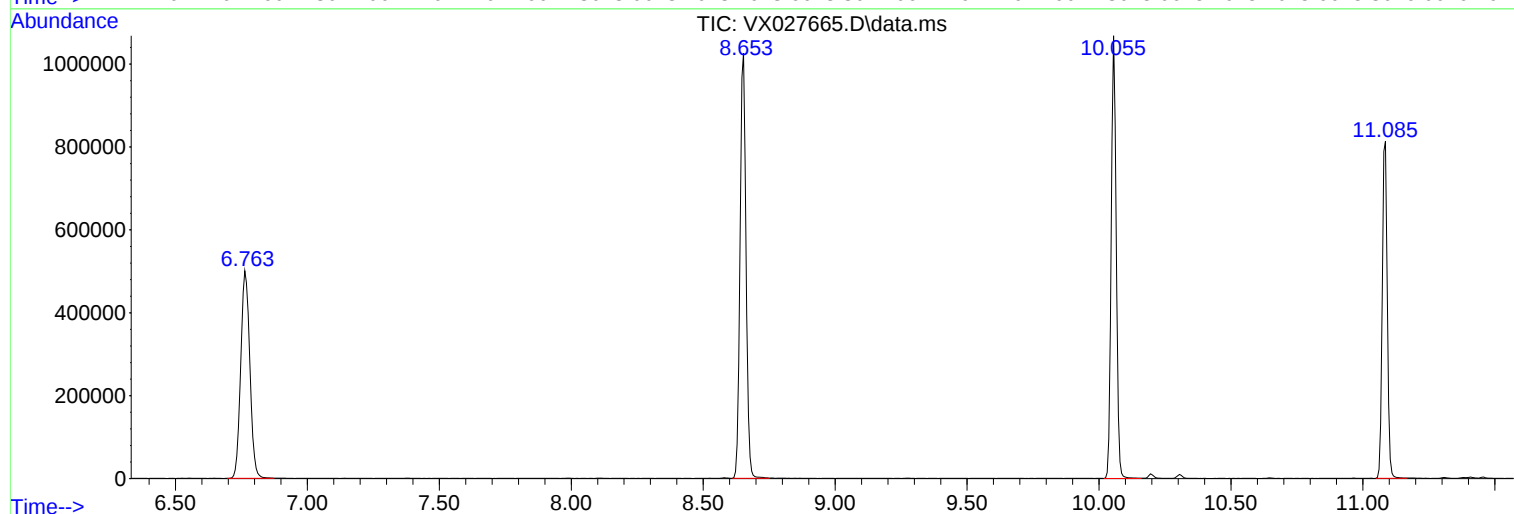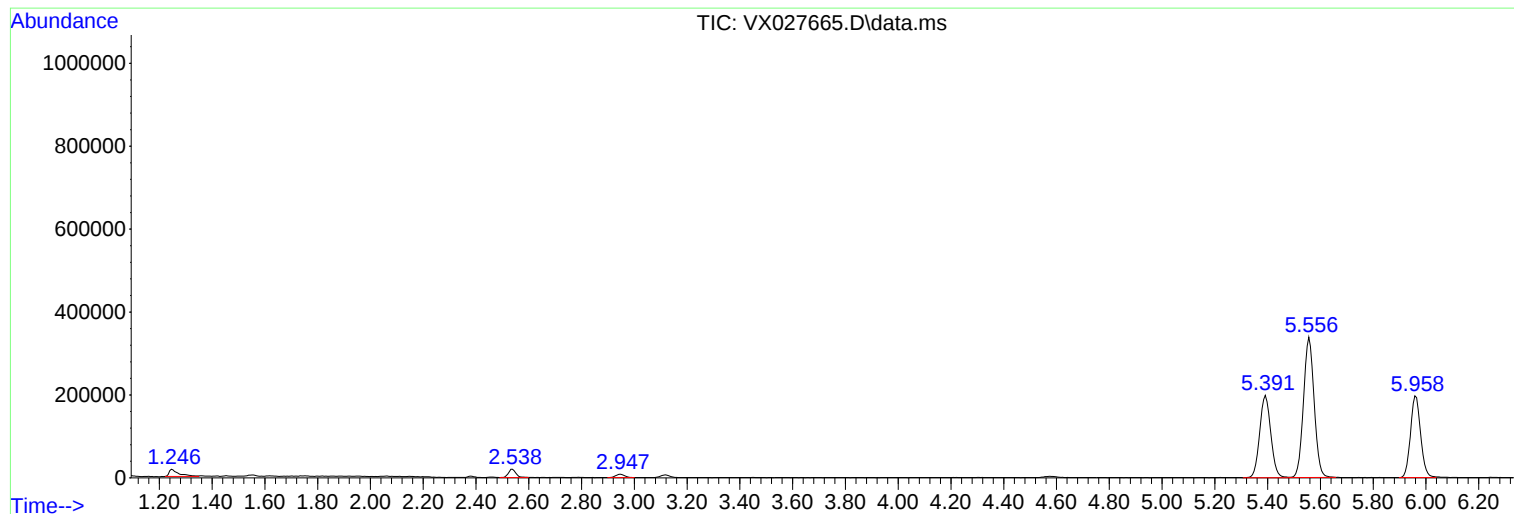

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032322\
Data File : VX027665.D
Acq On : 23 Mar 2022 14:16
Operator : JC/MD
Sample : N2028-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-116D

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032322\
Data File : VX027665.D
Acq On : 23 Mar 2022 14:16
Operator : JC/MD
Sample : N2028-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-116D

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------