

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032322\
 Data File : VX027679.D
 Acq On : 23 Mar 2022 20:09
 Operator : JC/MD
 Sample : N2028-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-118E

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
 Title : SW846 8260

Signal : TIC: VX027679.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	22	27	33	rBV2	9934	24957	1.49%	0.277%
2	2.538	230	238	248	rBV	11774	23051	1.38%	0.256%
3	3.117	325	333	343	rVB	9488	22120	1.32%	0.246%
4	5.391	693	706	722	rBV	206405	598088	35.75%	6.640%
5	5.556	722	733	754	rVB	349017	986482	58.96%	10.952%
6	5.958	788	799	818	rBV	202121	545708	32.62%	6.059%
7	6.763	921	931	944	rBV	523499	1240616	74.15%	13.774%
8	8.653	1234	1241	1252	rBV	1063098	1673107	100.00%	18.575%
9	10.055	1465	1471	1485	rBV	1094908	1454436	86.93%	16.148%
10	11.079	1634	1639	1655	rBV	862733	1111706	66.45%	12.342%
11	12.024	1788	1794	1808	rBV	1067493	1326884	79.31%	14.731%




Sum of corrected areas: 9007155

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032322\
Data File : VX027679.D
Acq On : 23 Mar 2022 20:09
Operator : JC/MD
Sample : N2028-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-118E

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

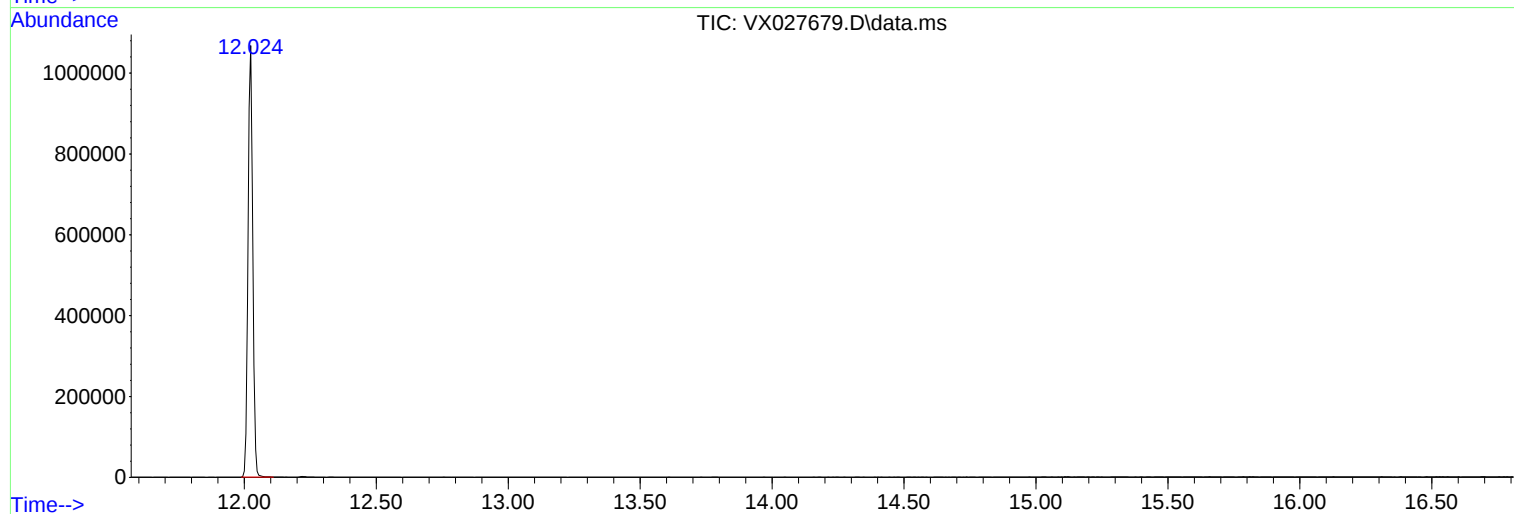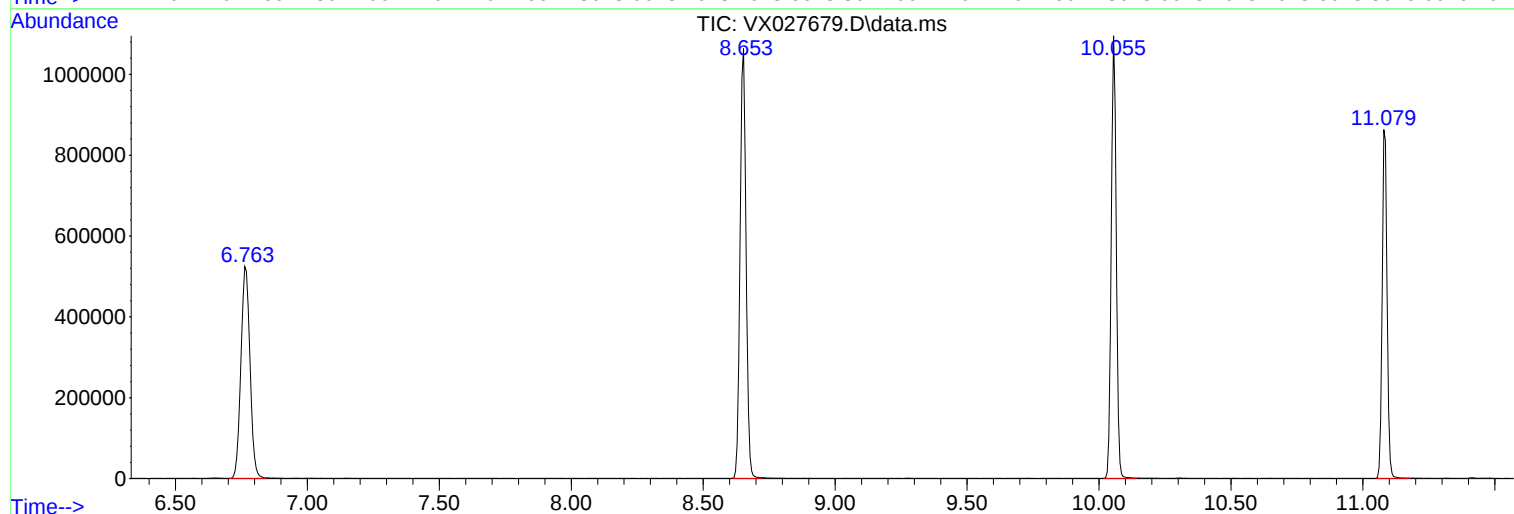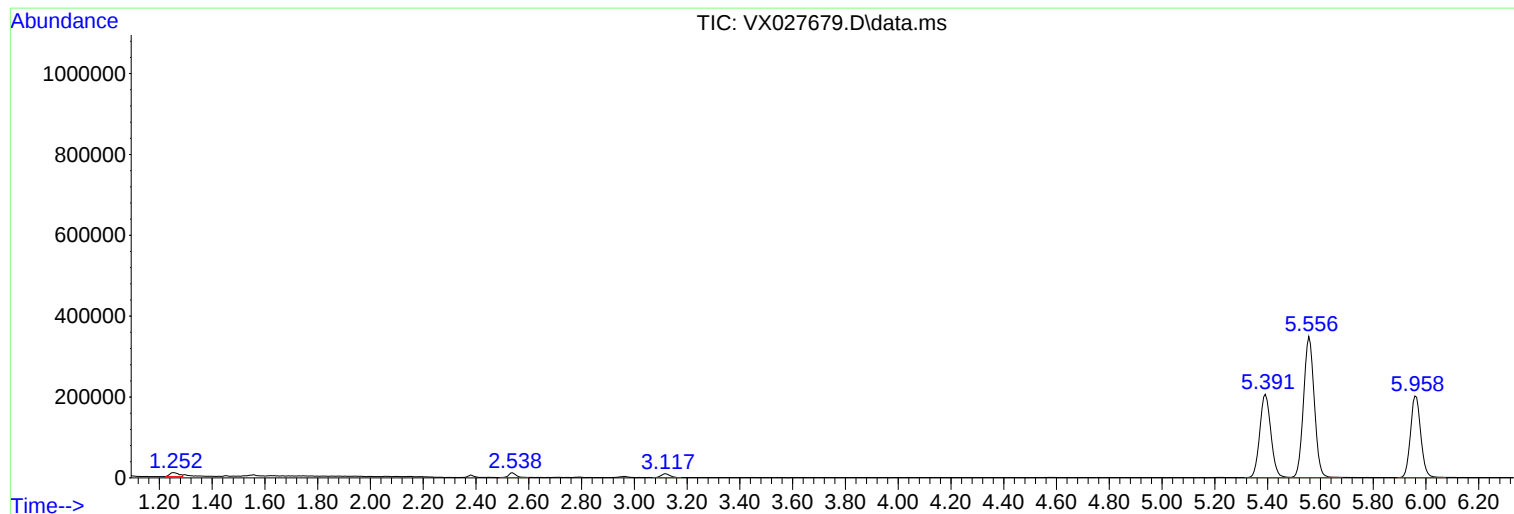

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032322\
Data File : VX027679.D
Acq On : 23 Mar 2022 20:09
Operator : JC/MD
Sample : N2028-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-118E

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032322\
Data File : VX027679.D
Acq On : 23 Mar 2022 20:09
Operator : JC/MD
Sample : N2028-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-118E

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------