

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032322\
 Data File : VX027680.D
 Acq On : 23 Mar 2022 20:32
 Operator : JC/MD
 Sample : N2028-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-116

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M

Title : SW846 8260

Signal : TIC: VX027680.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	19	27	32	rBV2	10284	24048	1.46%	0.272%
2	2.538	230	238	246	rBV	21118	40005	2.43%	0.452%
3	5.099	646	658	670	rBV3	7369	22416	1.36%	0.253%
4	5.391	694	706	720	rBV	203324	588263	35.79%	6.643%
5	5.556	720	733	748	rVB	343016	973390	59.22%	10.992%
6	5.958	789	799	813	rBV	199249	535829	32.60%	6.051%
7	6.763	921	931	949	rBV	514941	1224261	74.49%	13.825%
8	8.653	1233	1241	1261	rBV	1036009	1643625	100.00%	18.560%
9	10.055	1465	1471	1487	rBV	1100576	1446831	88.03%	16.338%
10	11.085	1634	1640	1652	rBV	819319	1088682	66.24%	12.294%
11	12.024	1788	1794	1813	rBV	1058728	1268225	77.16%	14.321%




Sum of corrected areas: 8855575

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032322\
Data File : VX027680.D
Acq On : 23 Mar 2022 20:32
Operator : JC/MD
Sample : N2028-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-116

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

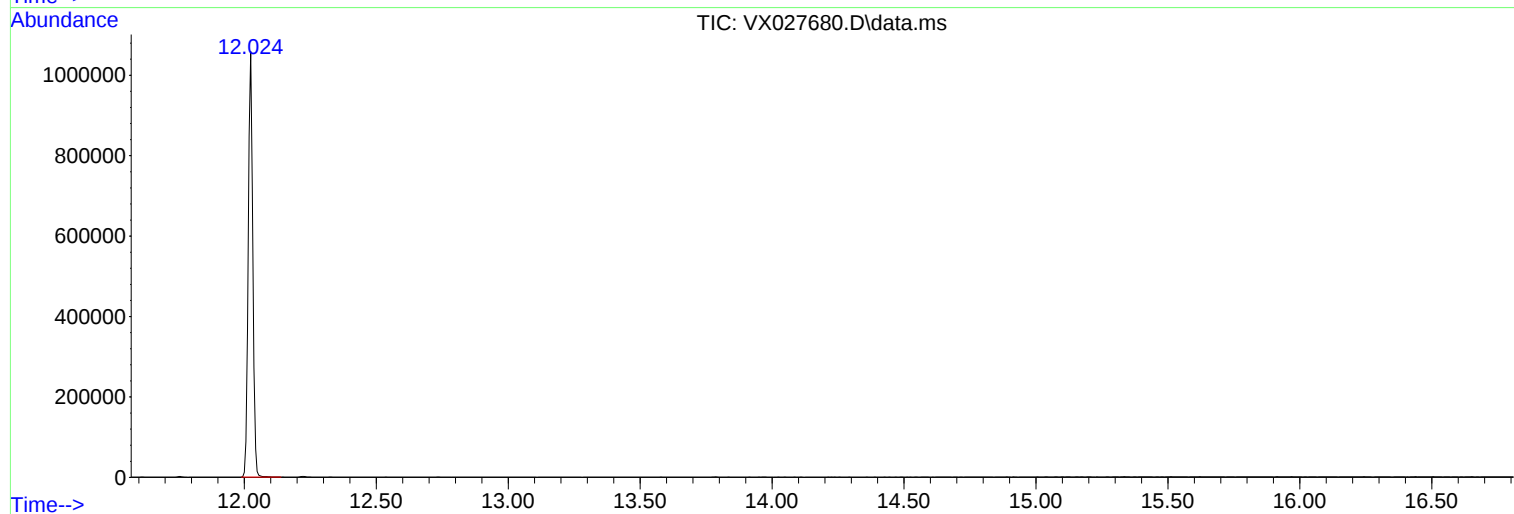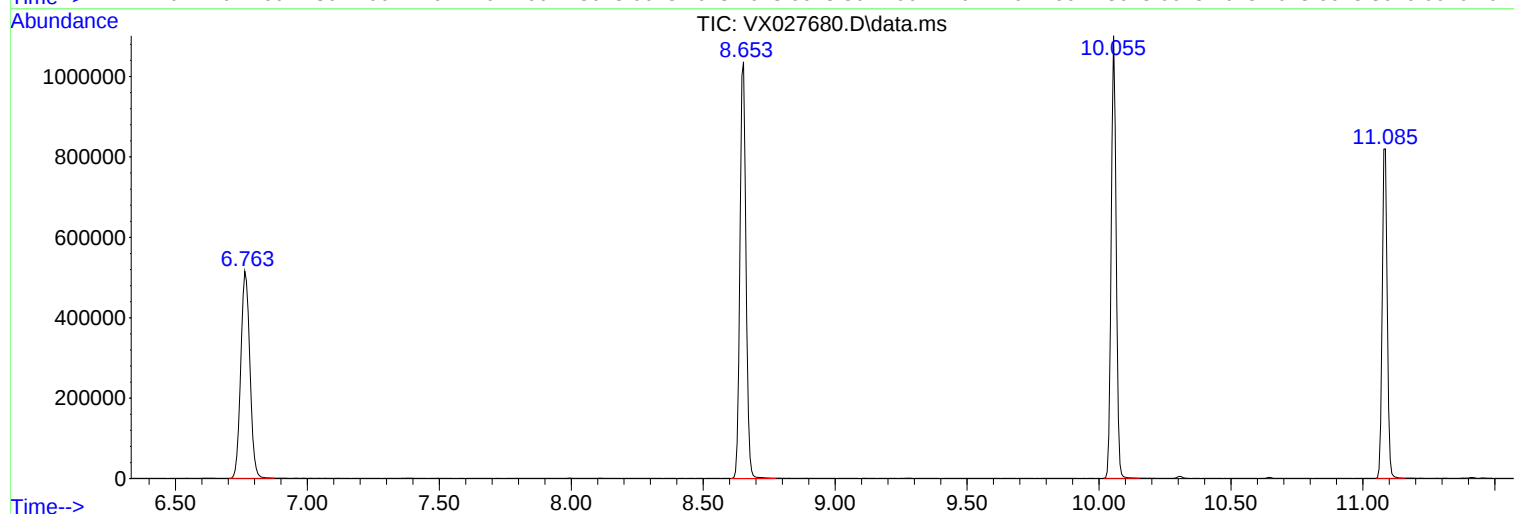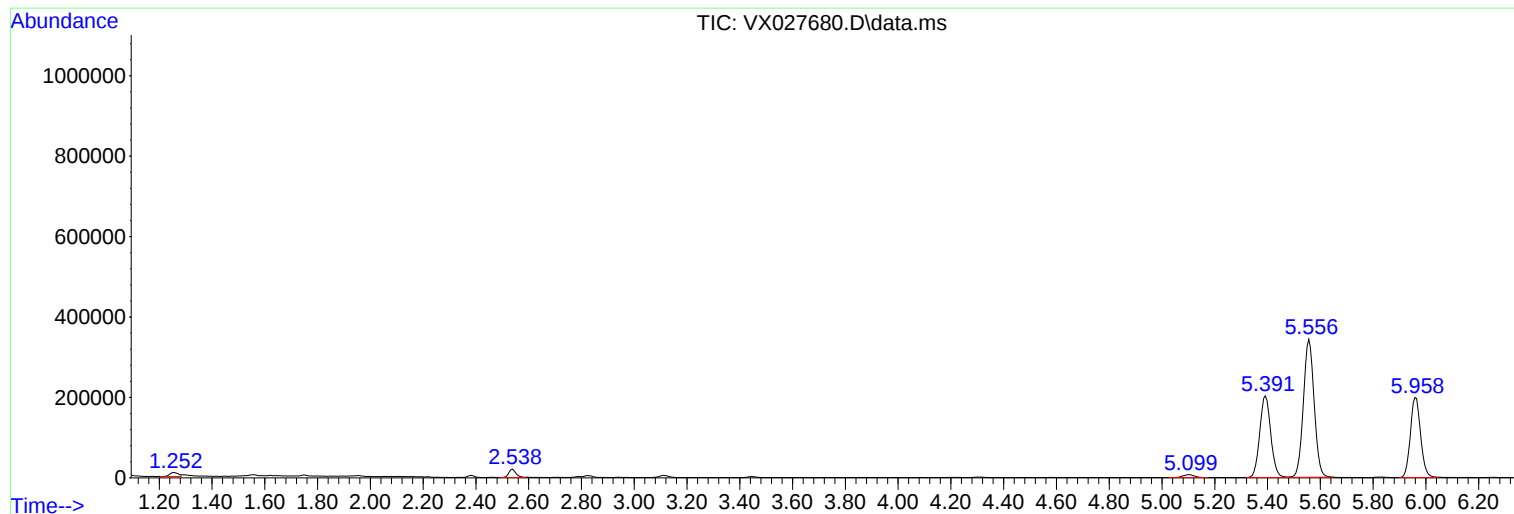

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032322\
Data File : VX027680.D
Acq On : 23 Mar 2022 20:32
Operator : JC/MD
Sample : N2028-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-116

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032322\
Data File : VX027680.D
Acq On : 23 Mar 2022 20:32
Operator : JC/MD
Sample : N2028-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-116

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------