
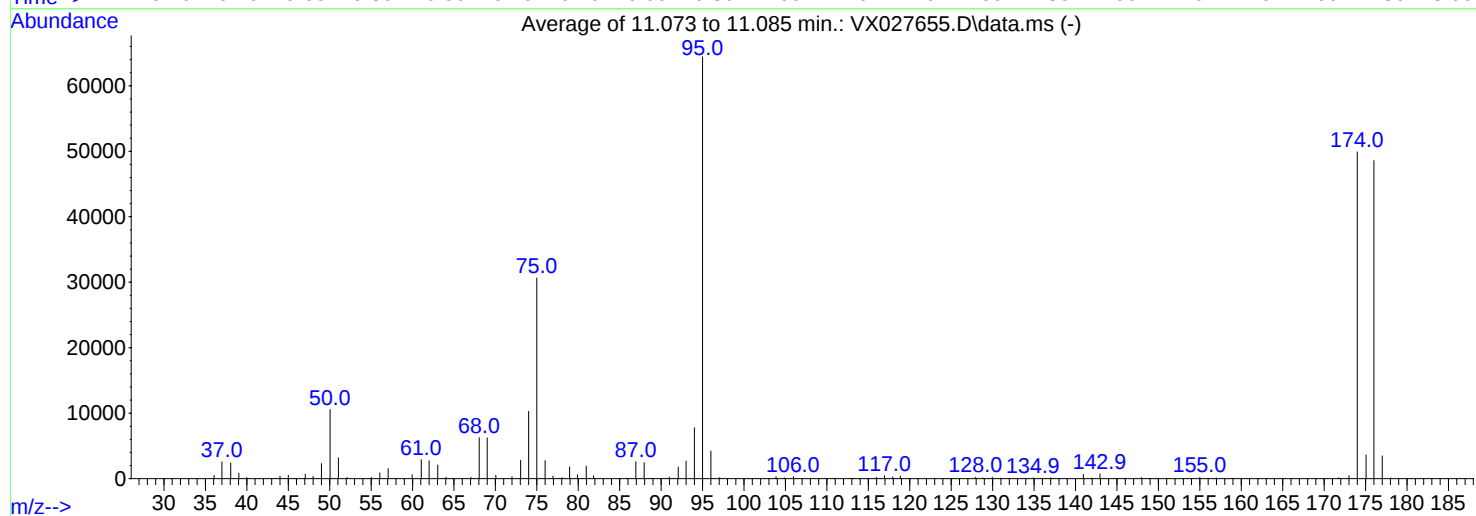


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX032322\  
 Data File : VX027655.D  
 Acq On : 23 Mar 2022 09:29  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031722W.M  
 Title : SW846 8260  
 Last Update : Thu Mar 17 15:02:59 2022

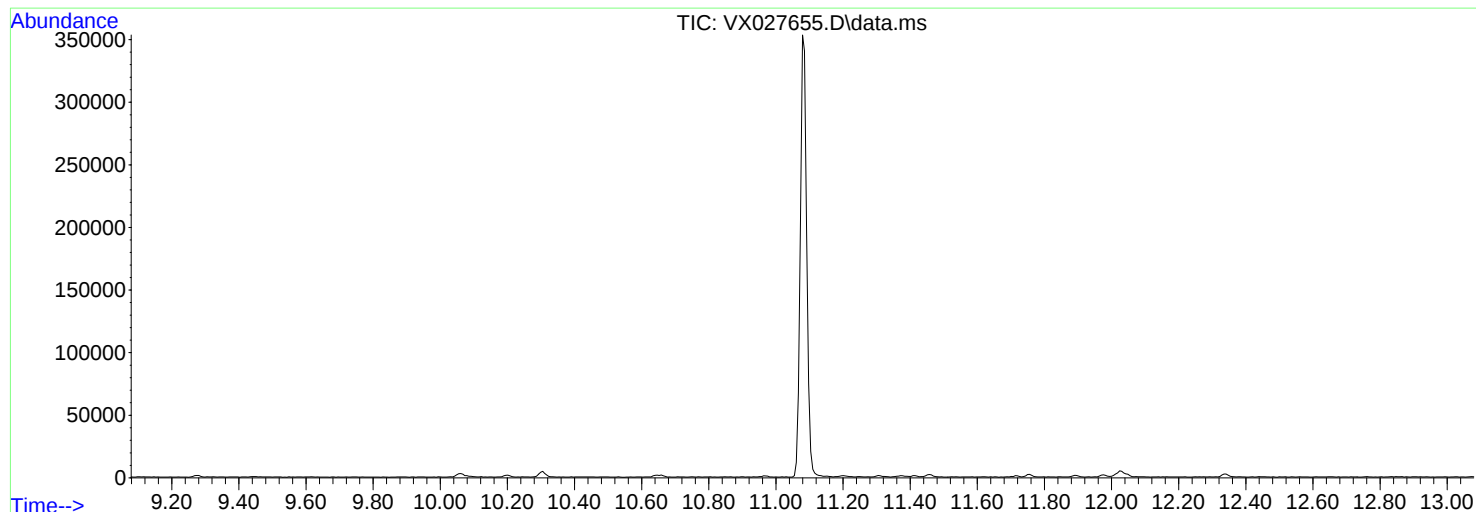

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 16.4         | 10565      | PASS                |
| 75             | 95              | 30              | 60              | 47.6         | 30659      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 64424      | PASS                |
| 96             | 95              | 5               | 9               | 6.5          | 4199       | PASS                |
| 173            | 174             | 0.00            | 2               | 0.9          | 470        | PASS                |
| 174            | 95              | 50              | 100             | 77.5         | 49899      | PASS                |
| 175            | 174             | 5               | 9               | 7.2          | 3611       | PASS                |
| 176            | 174             | 95              | 101             | 97.4         | 48587      | PASS                |
| 177            | 176             | 5               | 9               | 7.1          | 3461       | PASS                |