


Chloromethane

Response Ratio

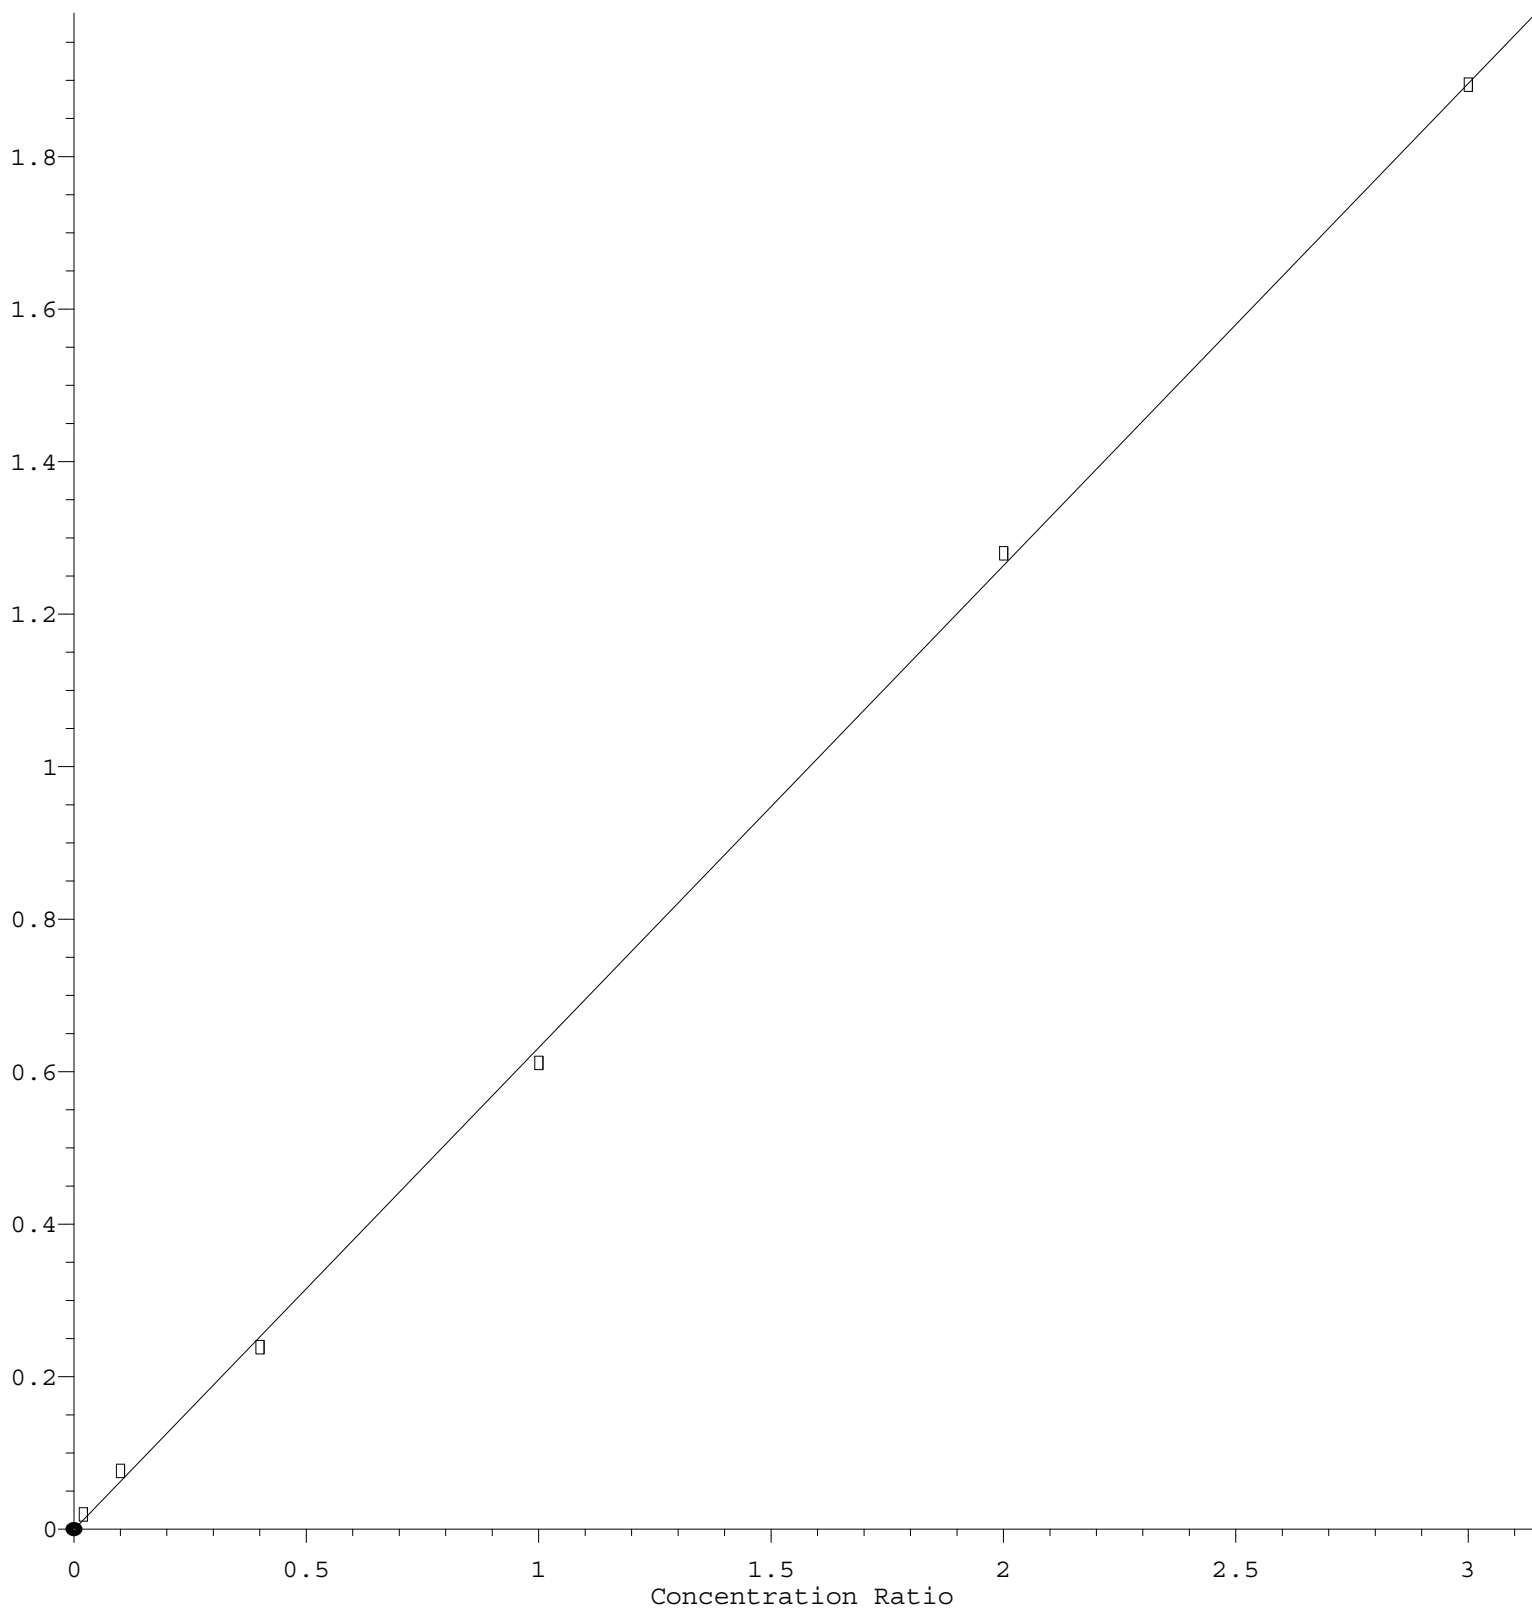

$$\text{Response} = 6.323\text{e-}001 * \text{Amt} - 5.327\text{e-}004$$


Coef of Det (r^2) = 0.999617 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X032421W.M

Calibration Table Last Updated: Wed Mar 24 12:25:26 2021

Methyl Iodide

Response Ratio

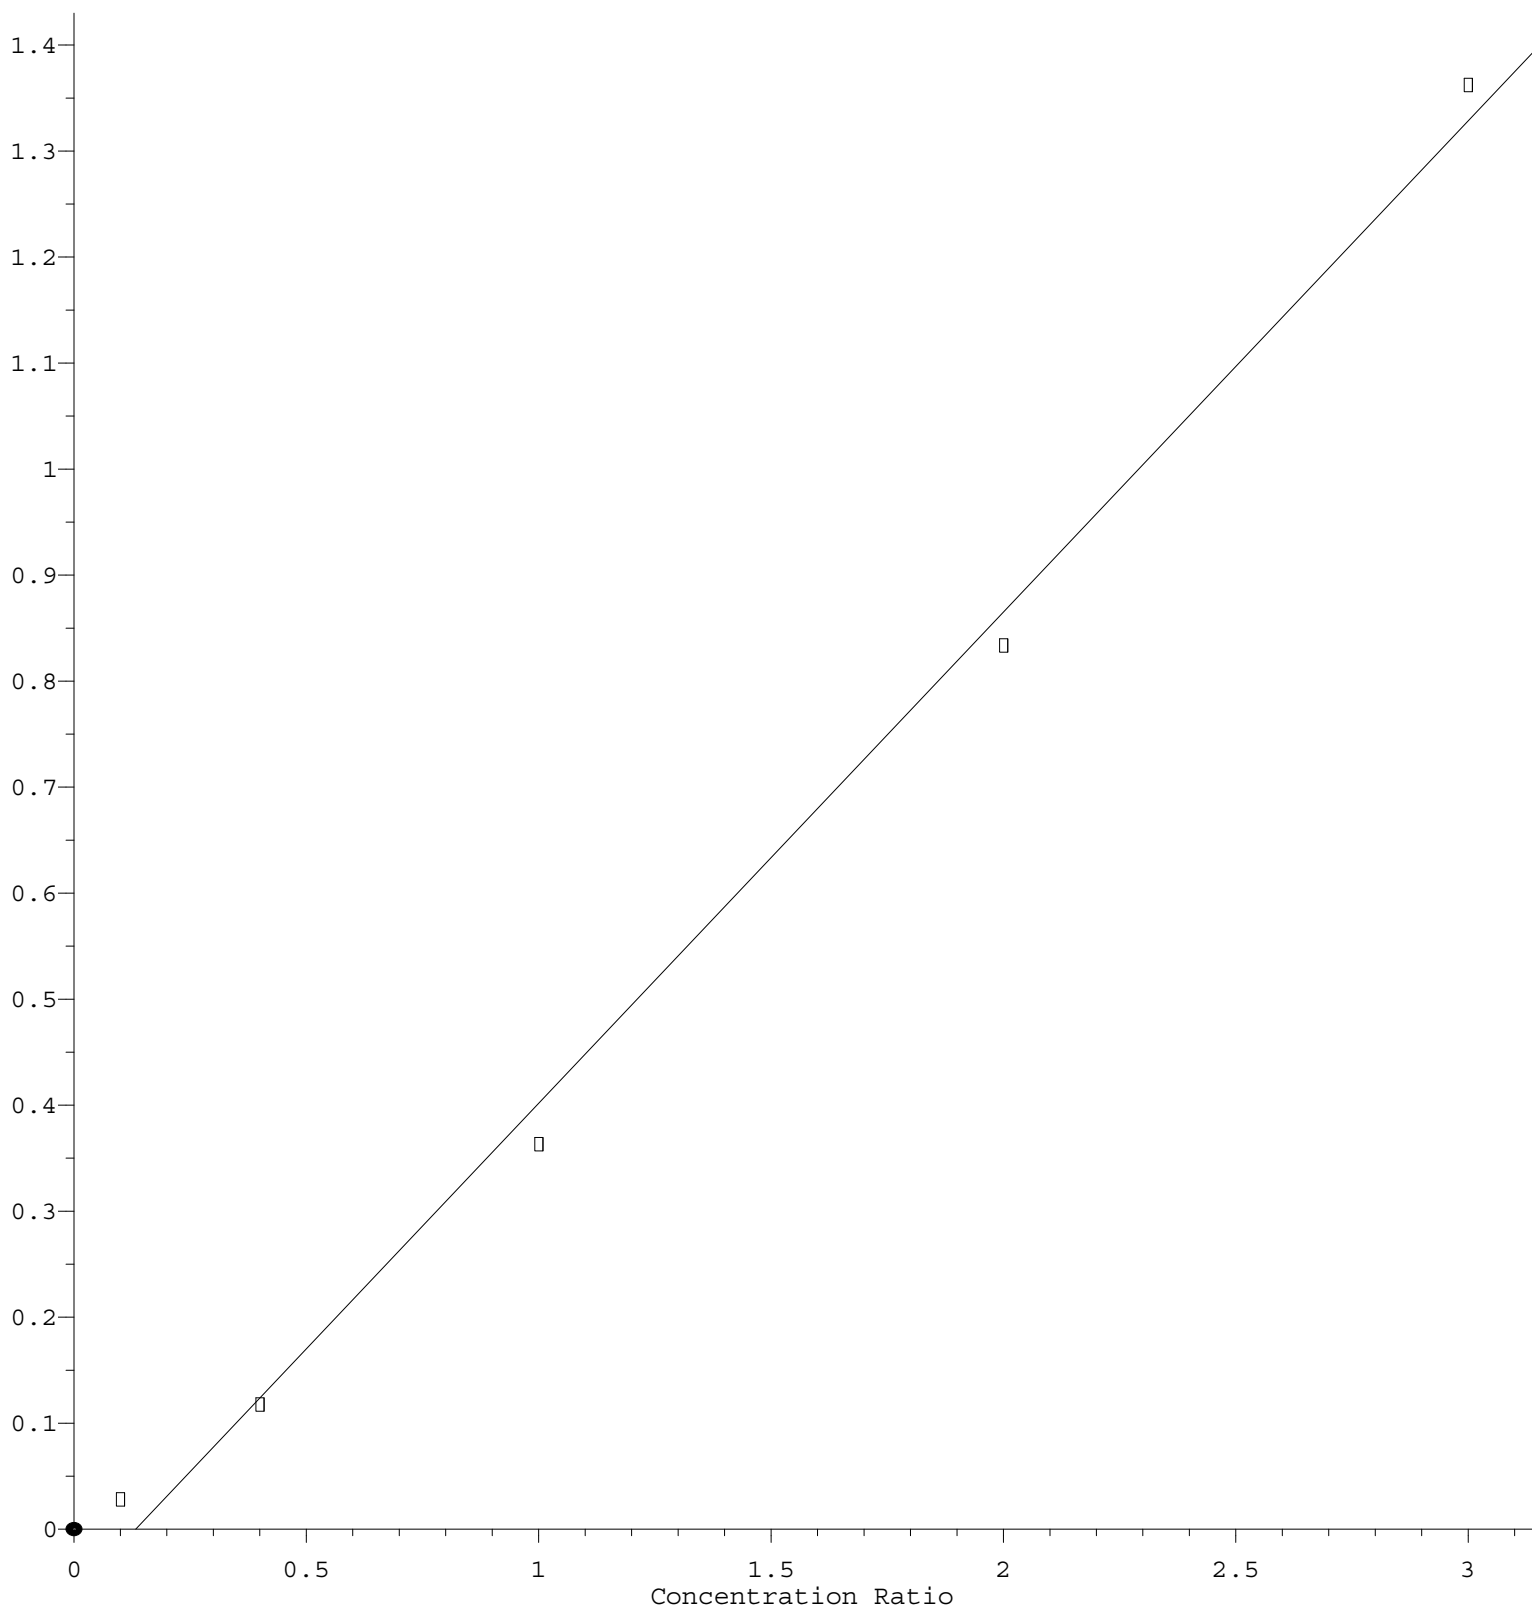

$$\text{Response} = 4.634\text{e-}001 * \text{Amt} - 6.156\text{e-}002$$


Coef of Det (r^2) = 0.995507 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X032421W.M

Calibration Table Last Updated: Wed Mar 24 12:25:26 2021

Acrolein

Response Ratio

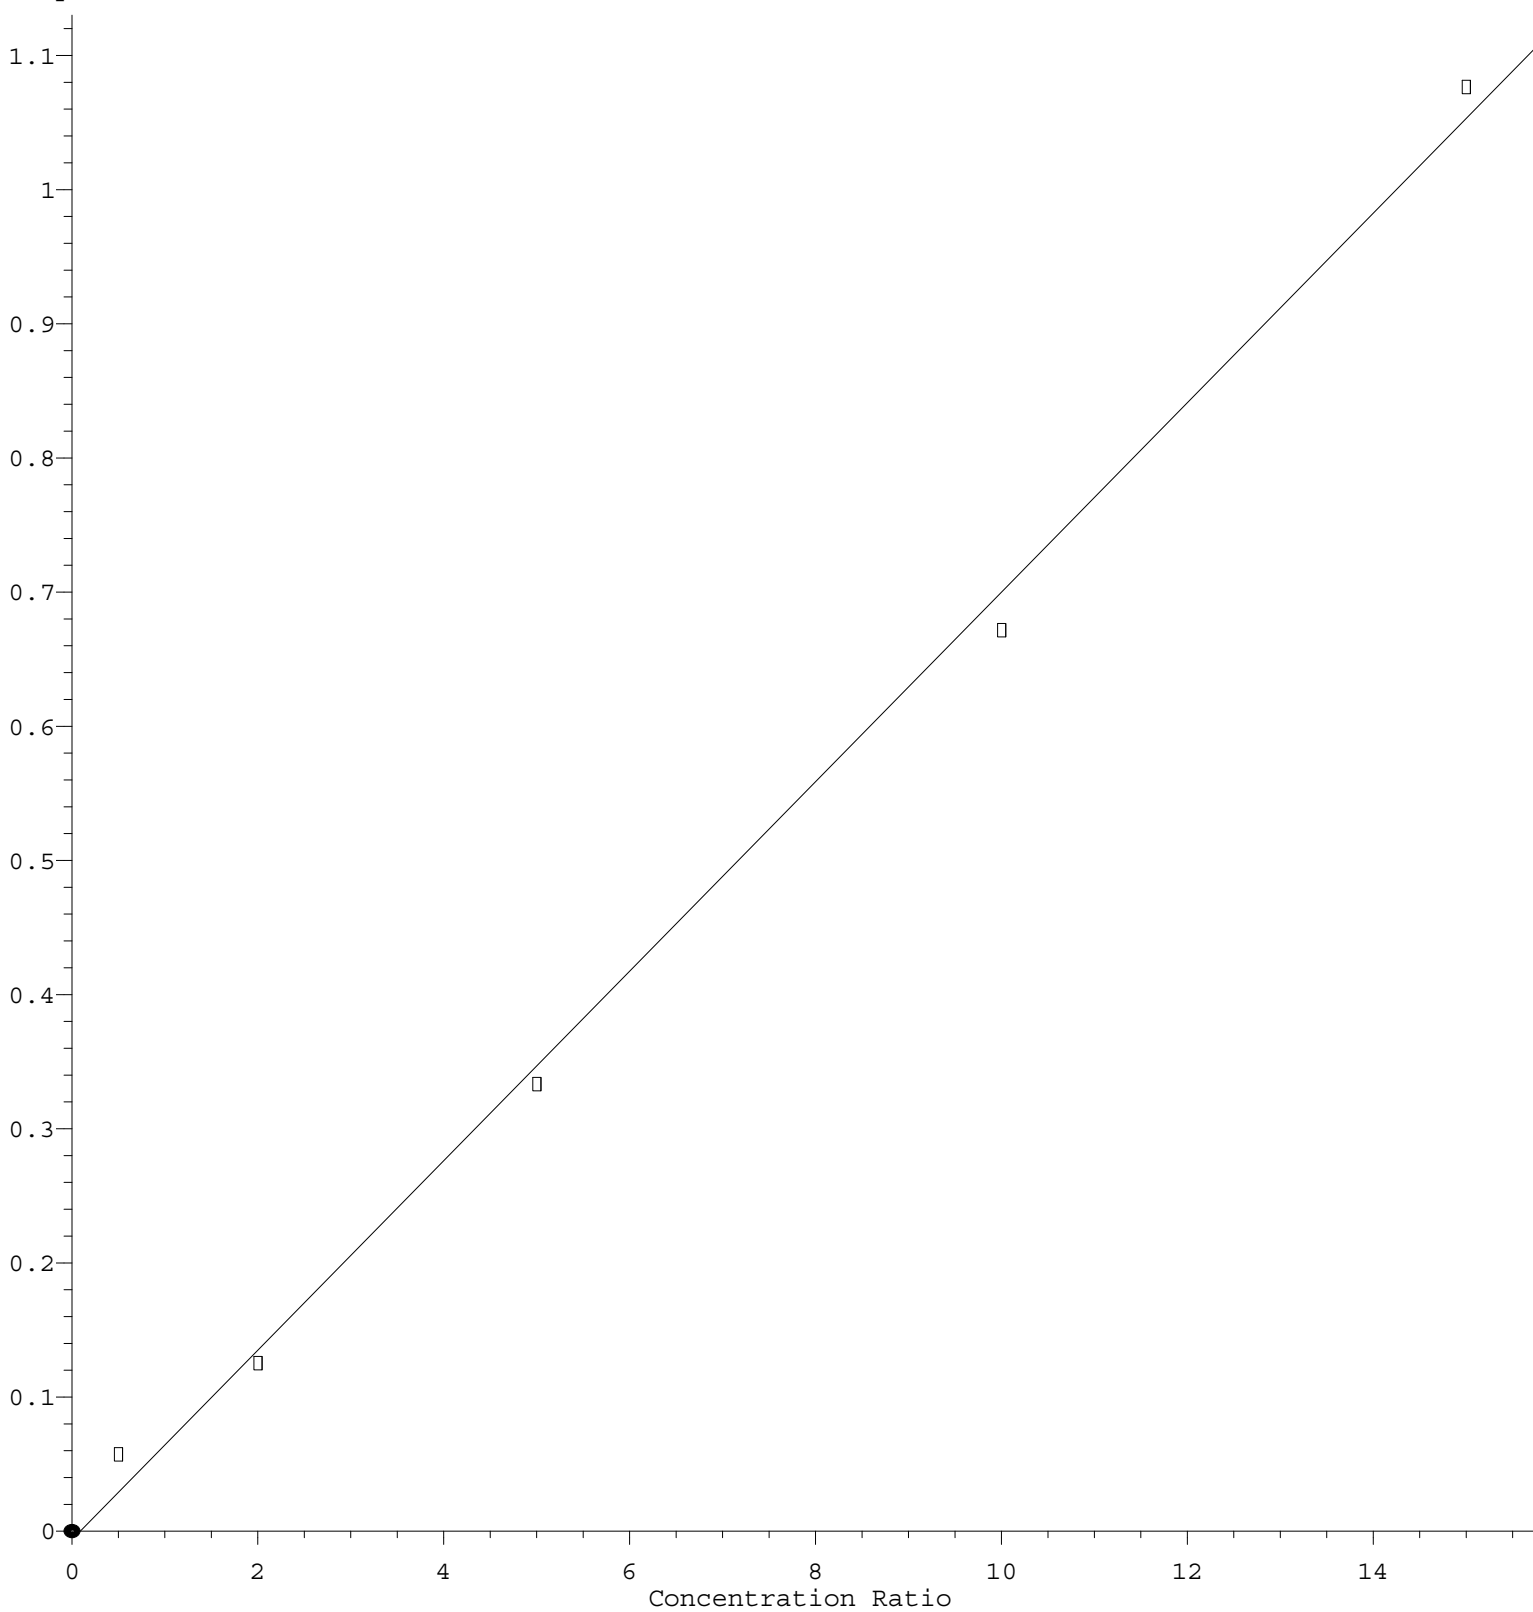

$$\text{Response} = 7.059\text{e-}002 * \text{Amt} - 6.067\text{e-}003$$


Coef of Det (r^2) = 0.996606 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X032421W.M

Calibration Table Last Updated: Wed Mar 24 12:25:26 2021

Ethyl methacrylate

Response Ratio

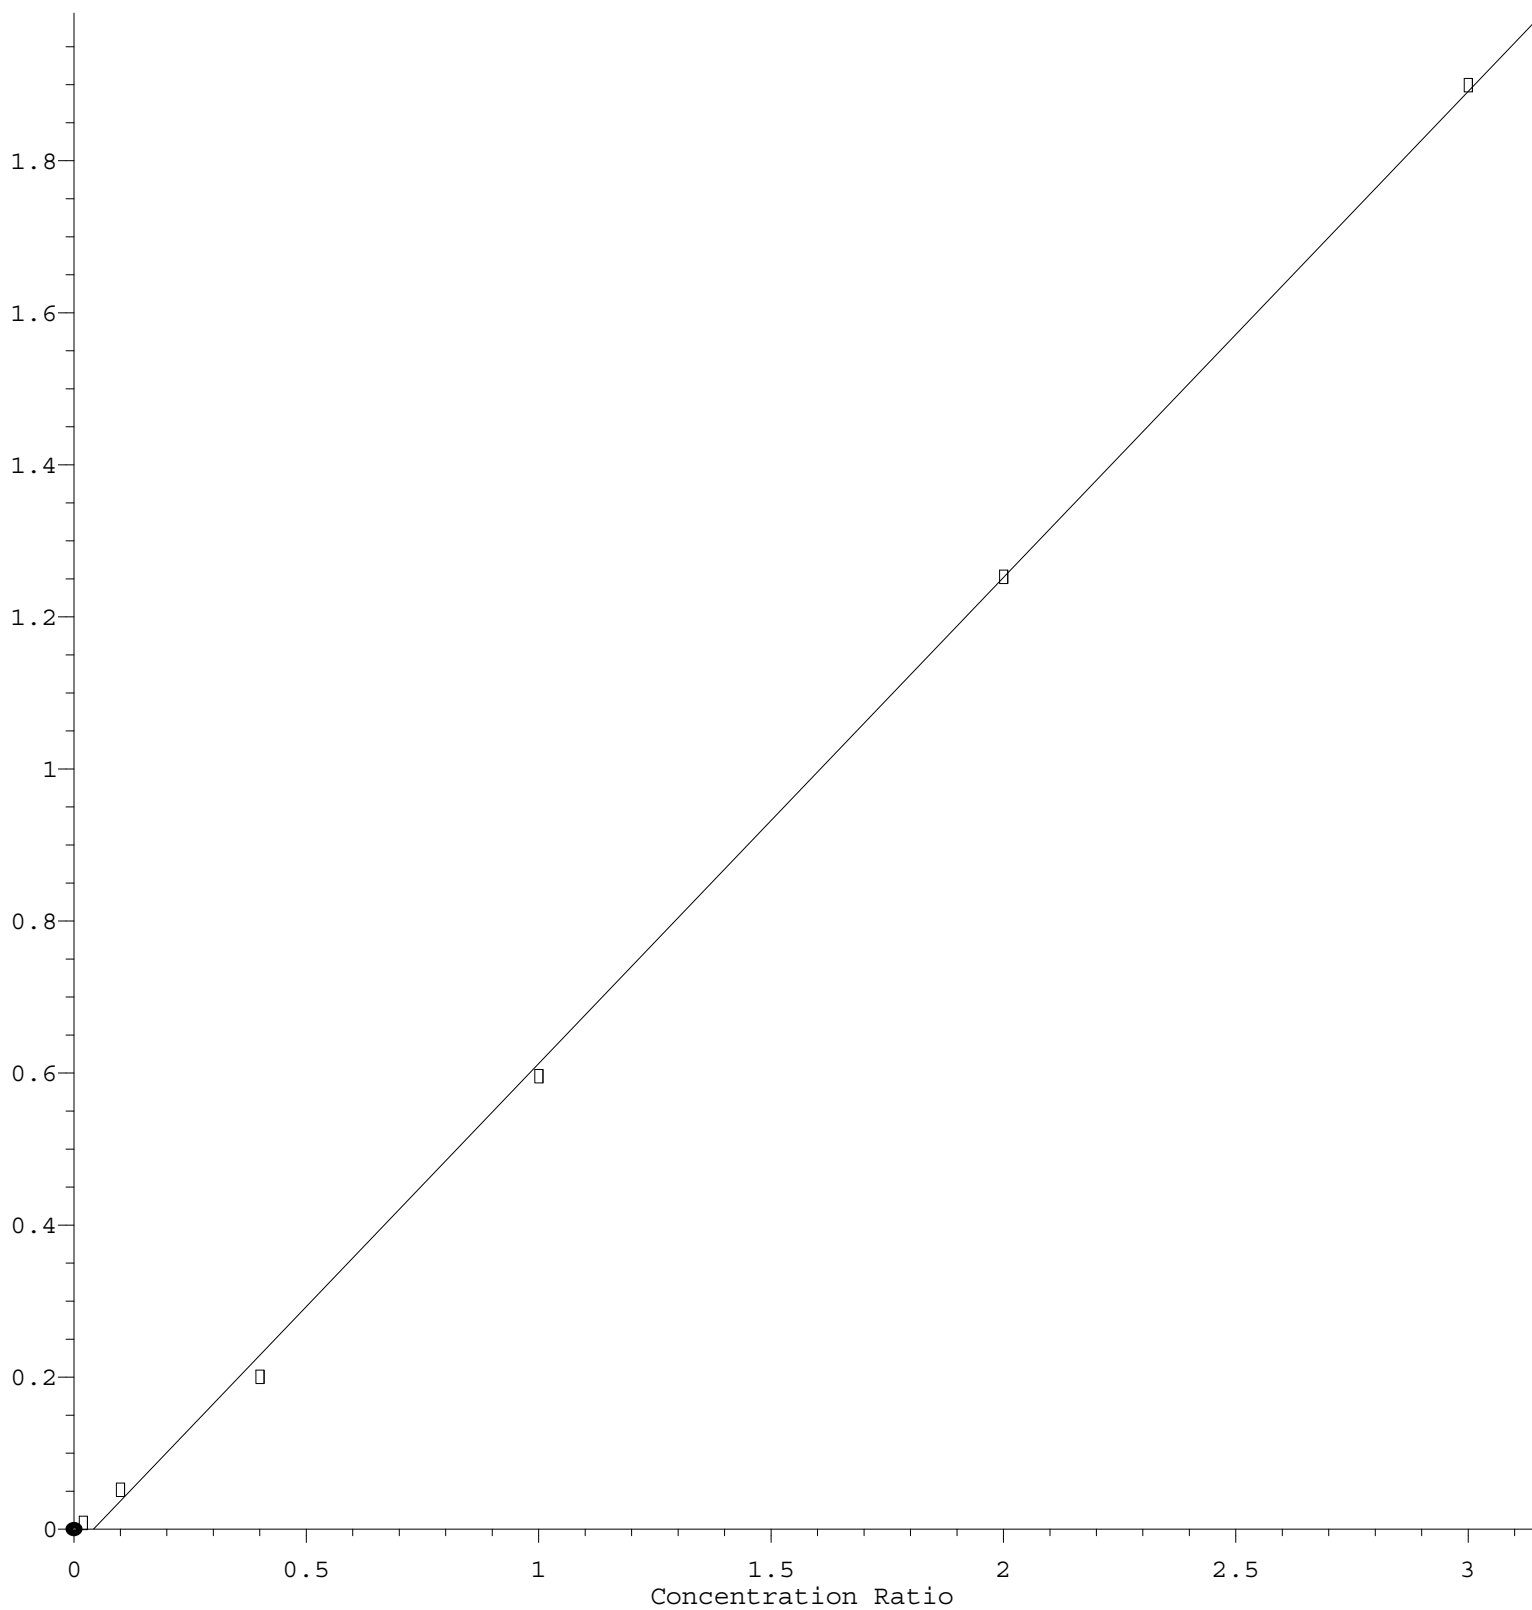

$$\text{Response} = 6.392\text{e-}001 * \text{Amt} - 2.660\text{e-}002$$


Coef of Det (r^2) = 0.999351 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X032421W.M

Calibration Table Last Updated: Wed Mar 24 12:25:26 2021

1,2-Dibromo-3-Chloropropane

Response Ratio

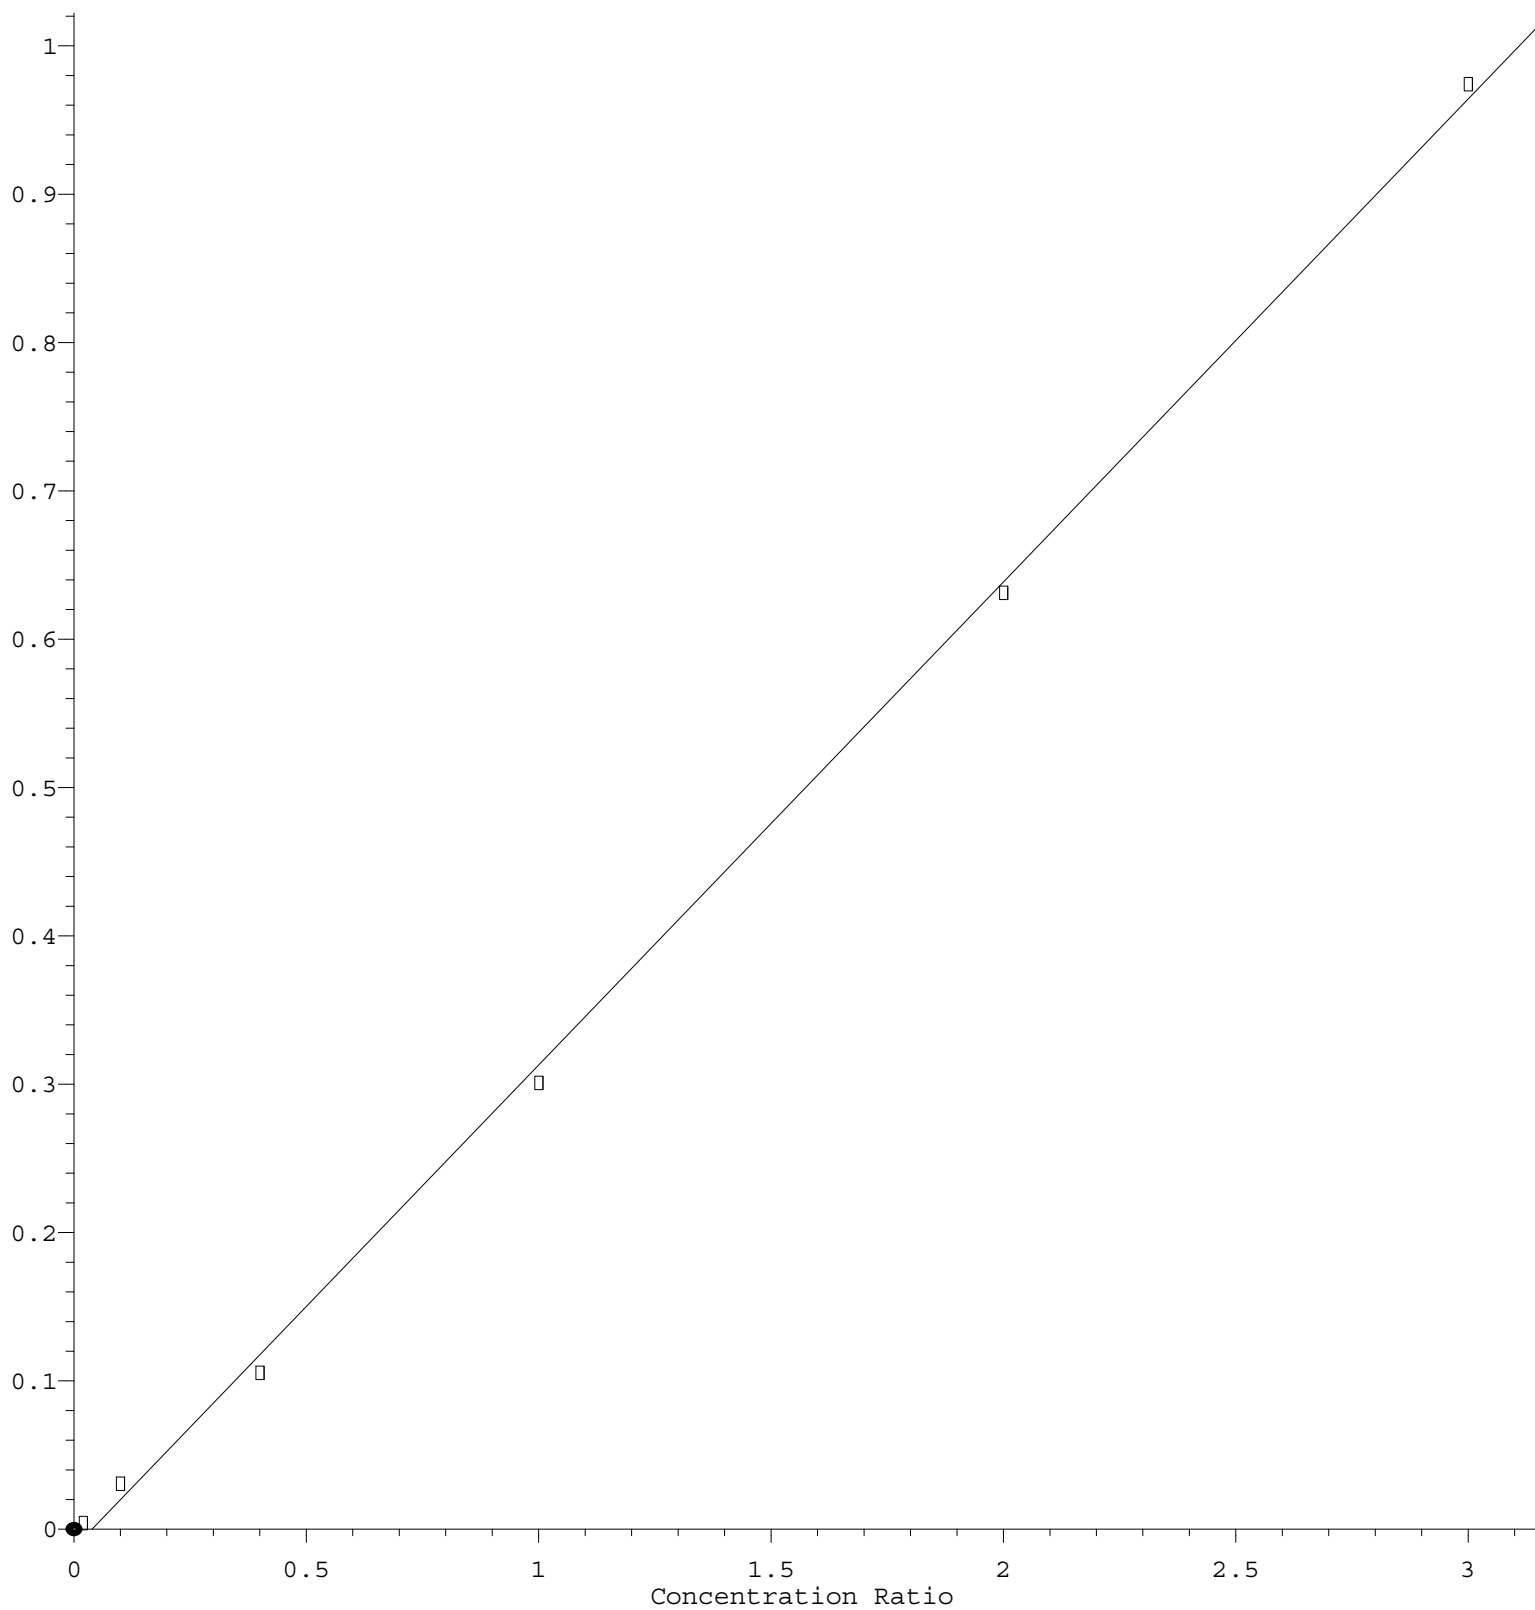

$$\text{Response} = 3.256\text{e-}001 * \text{Amt} - 1.282\text{e-}002$$

Coef of Det (r^2) = 0.999108 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X032421W.M

Calibration Table Last Updated: Wed Mar 24 12:25:26 2021