

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032421\
 Data File : VX021438.D
 Acq On : 24 Mar 2021 16:10
 Operator : JC/MD
 Sample : M1735-10 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE132D6-20210315

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M

Title : SW846 8260

Signal : TIC: VX021438.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.476	62	66	72	rBV	5409	7349	1.10%	0.240%
2	2.358	209	216	223	rBV6	5598	11181	1.67%	0.365%
3	5.470	733	745	758	rBV	51200	146592	21.87%	4.787%
4	5.629	761	772	785	rBV	79750	220296	32.86%	7.193%
5	6.035	830	841	852	rBV	56945	149719	22.33%	4.889%
6	6.835	963	977	990	rBV	130468	309389	46.15%	10.102%
7	7.188	1027	1037	1049	rBV	317410	670426	100.00%	21.891%
8	8.694	1285	1293	1302	rBV	269762	429862	64.12%	14.036%
9	10.094	1525	1531	1547	rVB	299025	409869	61.14%	13.383%
10	11.118	1699	1705	1716	rBV	252586	324380	48.38%	10.592%
11	12.059	1859	1865	1876	rBV	309580	383496	57.20%	12.522%




Sum of corrected areas: 3062559

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032421\
Data File : VX021438.D
Acq On : 24 Mar 2021 16:10
Operator : JC/MD
Sample : M1735-10 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D6-20210315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

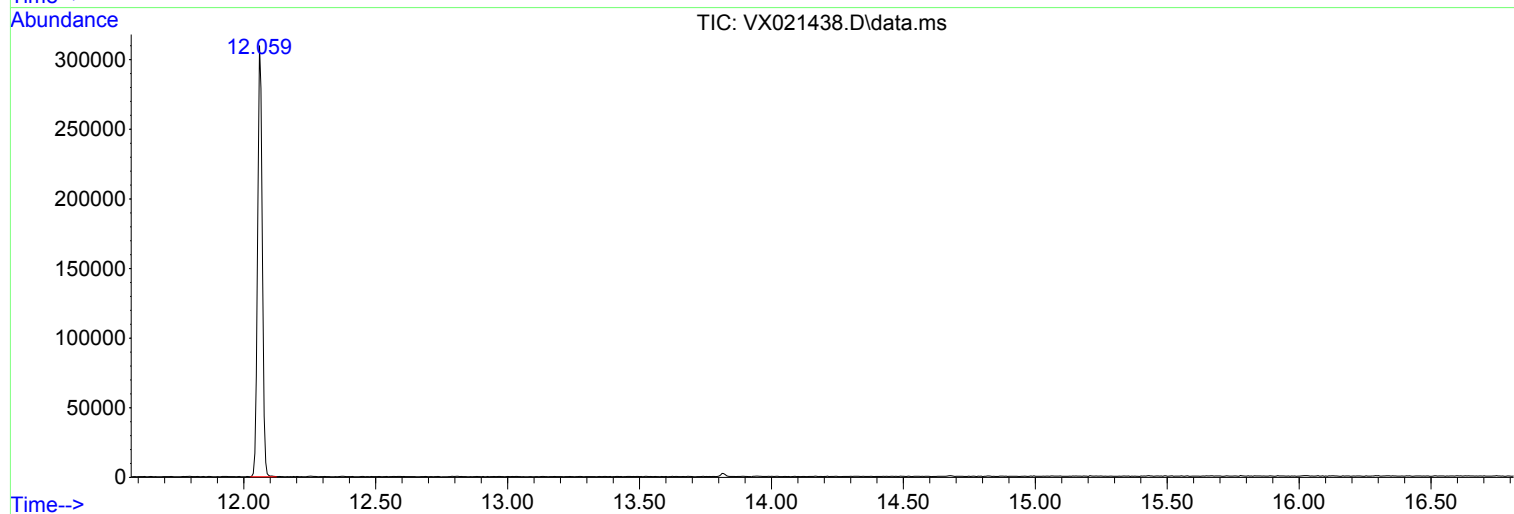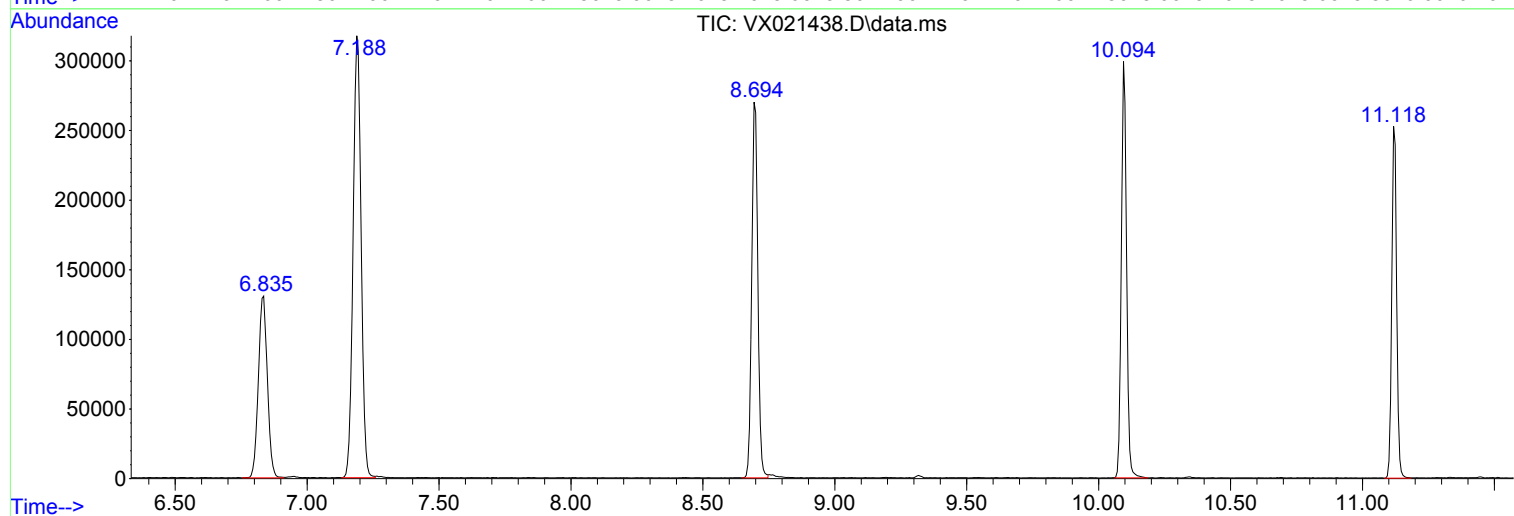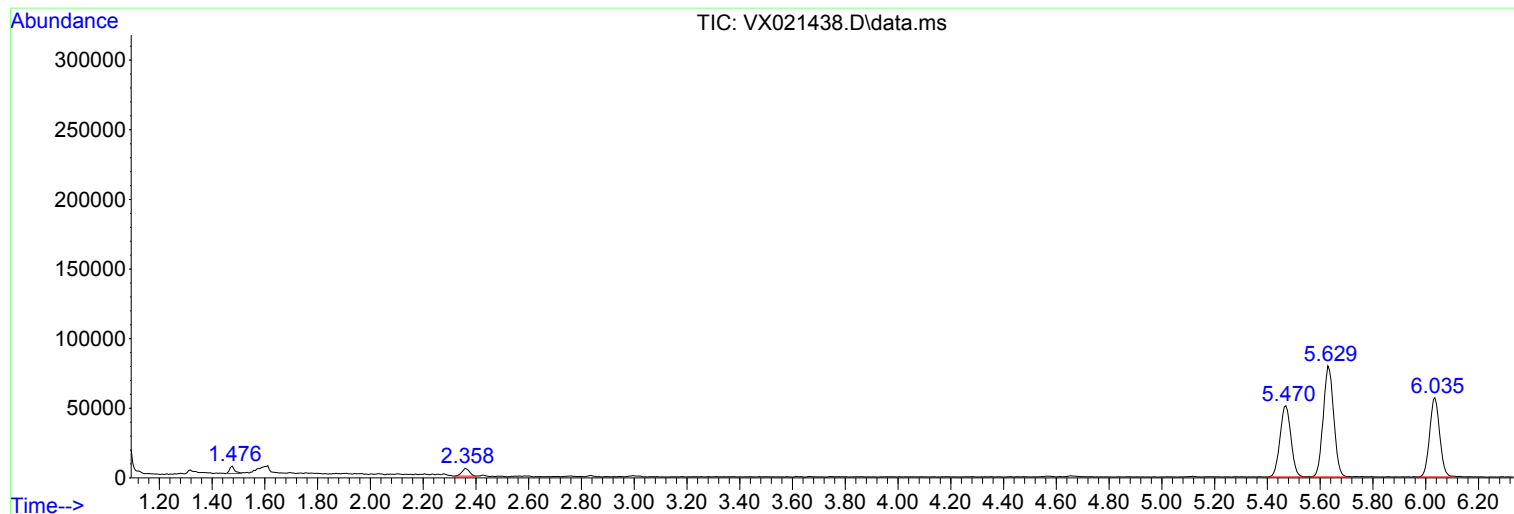

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032421\
Data File : VX021438.D
Acq On : 24 Mar 2021 16:10
Operator : JC/MD
Sample : M1735-10 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D6-20210315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032421\
Data File : VX021438.D
Acq On : 24 Mar 2021 16:10
Operator : JC/MD
Sample : M1735-10 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D6-20210315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------