

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032421\
 Data File : VX021460.D
 Acq On : 25 Mar 2021 01:48
 Operator : JC/MD
 Sample : M1770-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-103I

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
 Title : SW846 8260

Signal : TIC: VX021460.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.587	79	85	89	rVB5	2762	4884	1.24%	0.222%
2	2.423	222	227	233	rBV	4007	6463	1.65%	0.294%
3	2.581	244	254	262	rBV	8314	16489	4.20%	0.750%
4	5.464	733	744	760	rVB	48842	139261	35.45%	6.337%
5	5.629	760	772	785	rBV	71932	200985	51.16%	9.146%
6	6.029	826	840	852	rBV	55419	142224	36.20%	6.472%
7	6.829	965	976	988	rBV	121809	284987	72.54%	12.969%
8	8.694	1286	1293	1307	rBV	253501	392859	100.00%	17.878%
9	10.094	1525	1531	1546	rVB	267688	371956	94.68%	16.927%
10	11.118	1700	1705	1715	rBV	217378	287771	73.25%	13.096%
11	12.059	1859	1865	1877	rBV	283425	345602	87.97%	15.727%
12	12.889	2001	2006	2013	rBV2	3059	3996	1.02%	0.182%




Sum of corrected areas: 2197477

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032421\
Data File : VX021460.D
Acq On : 25 Mar 2021 01:48
Operator : JC/MD
Sample : M1770-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-103I

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

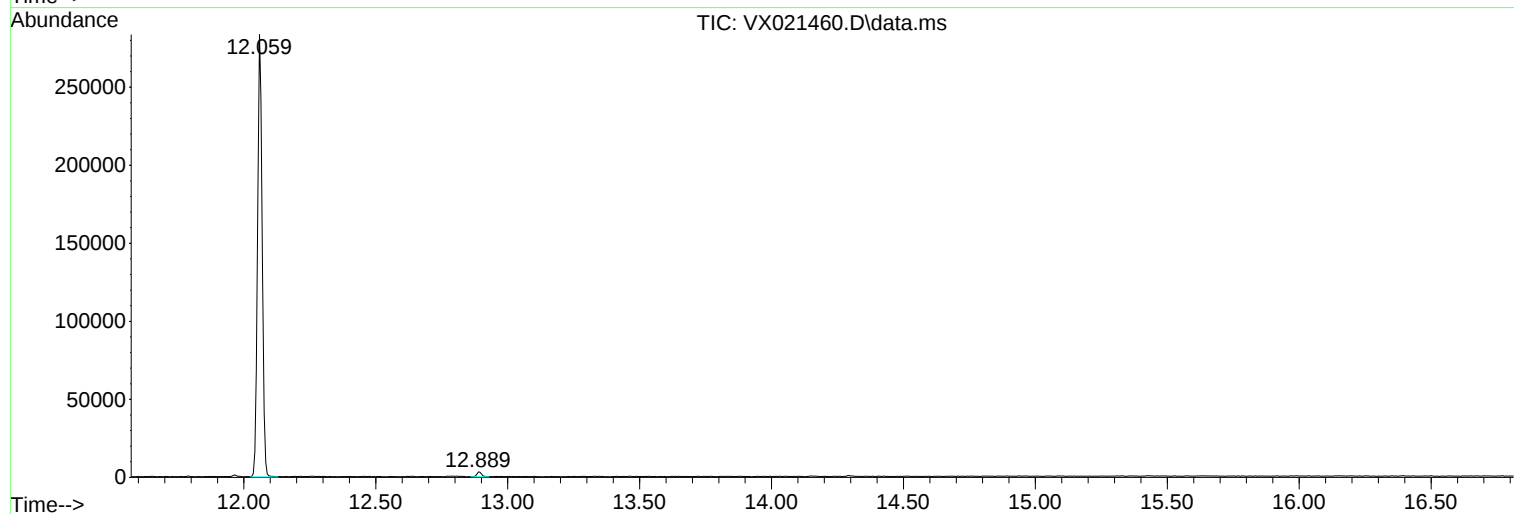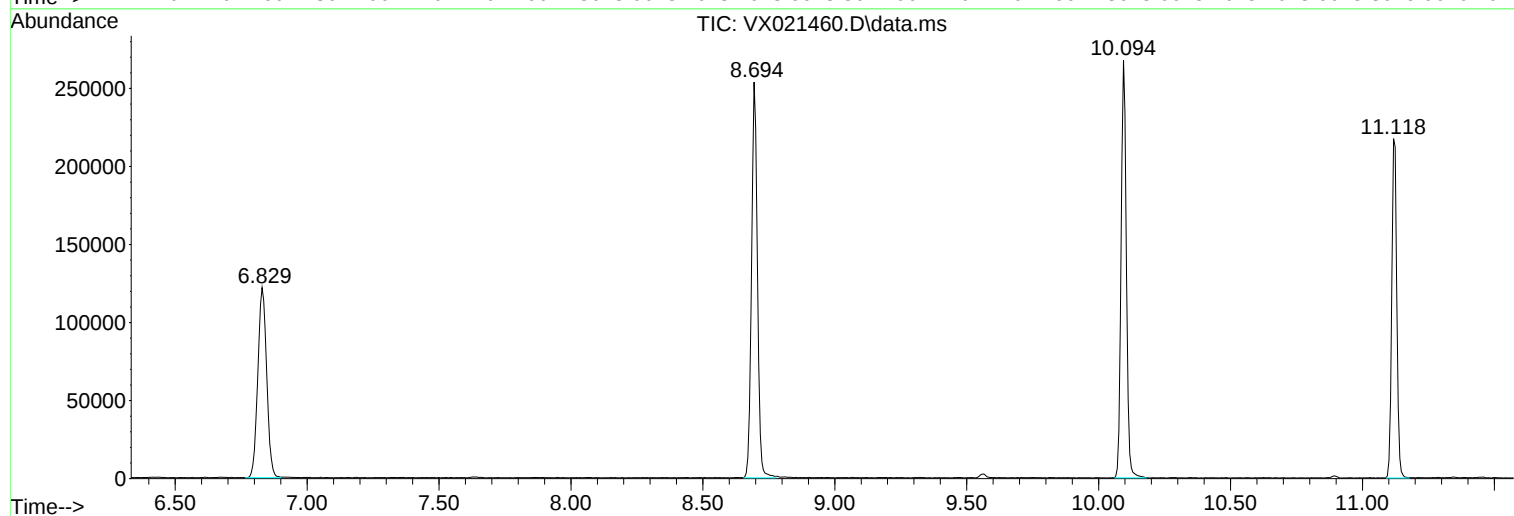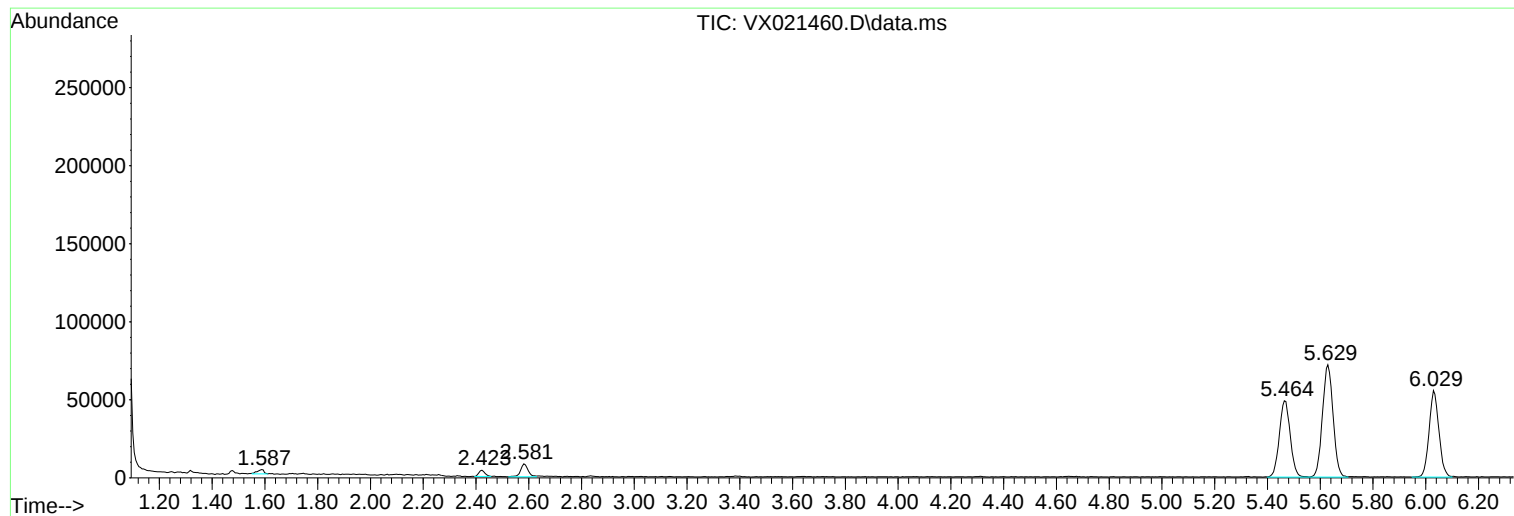

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032421\
Data File : VX021460.D
Acq On : 25 Mar 2021 01:48
Operator : JC/MD
Sample : M1770-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-103I

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032421\
Data File : VX021460.D
Acq On : 25 Mar 2021 01:48
Operator : JC/MD
Sample : M1770-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-103I

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------