
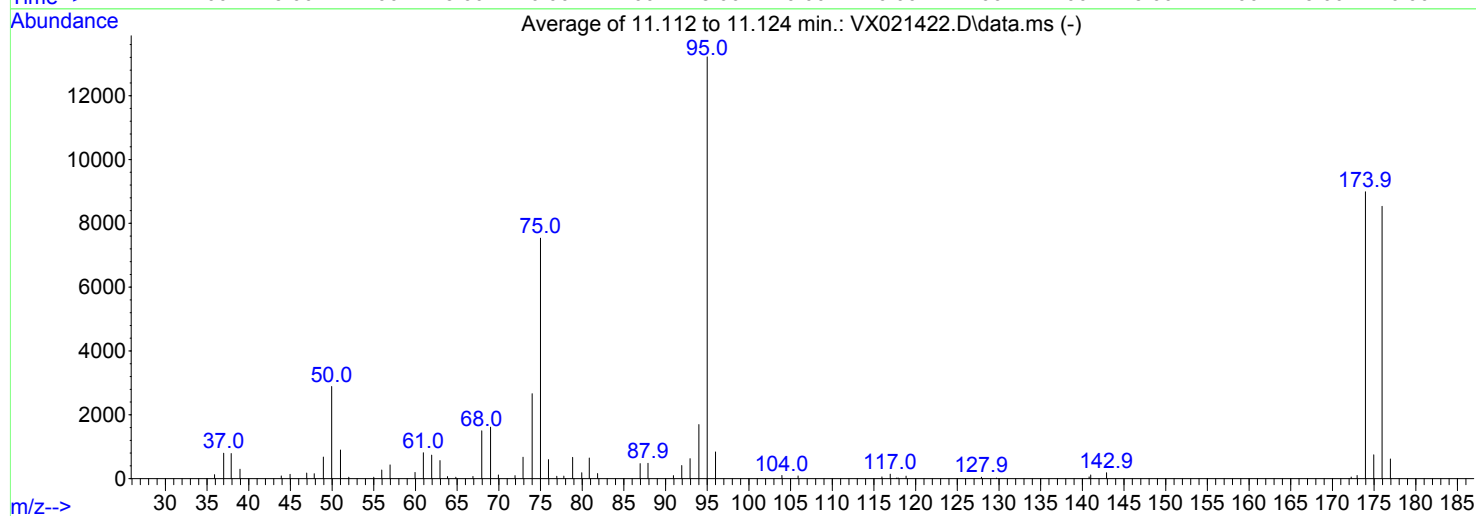


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032421\
 Data File : VX021422.D
 Acq On : 24 Mar 2021 08:21
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
 Title : SW846 8260
 Last Update : Wed Mar 24 12:25:26 2021

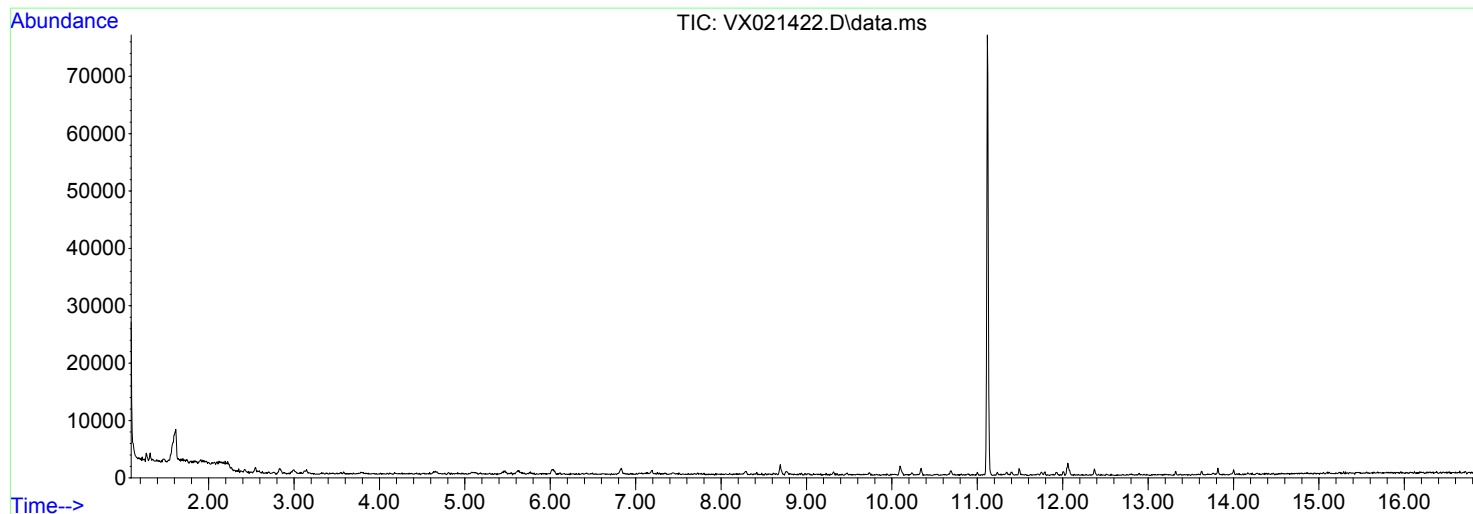

Spectrum Information: Average of 11.112 to 11.124 min.

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.9	2888	PASS
75	95	30	60	57.0	7536	PASS
95	95	100	100	100.0	13217	PASS
96	95	5	9	6.3	838	PASS
173	174	0.00	2	1.1	98	PASS
174	95	50	100	68.0	8991	PASS
175	174	5	9	8.3	746	PASS
176	174	95	101	94.9	8535	PASS
177	176	5	9	7.3	619	PASS