
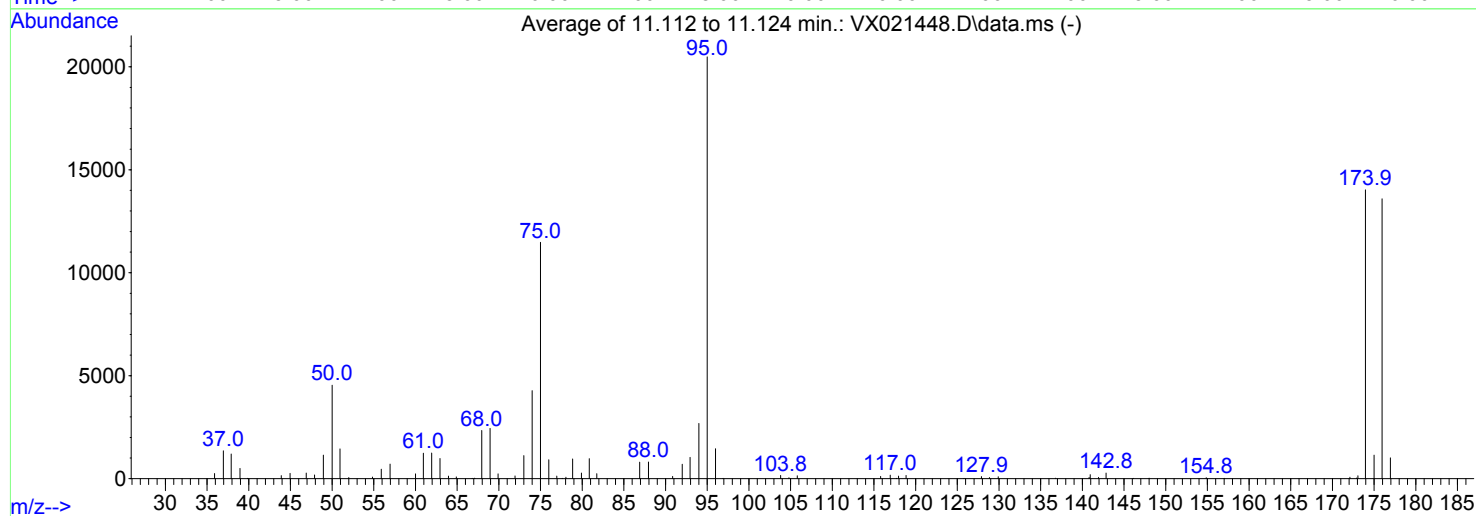


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032421\
Data File : VX021448.D
Acq On : 24 Mar 2021 20:43
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Title : SW846 8260
Last Update : Wed Mar 24 12:25:26 2021

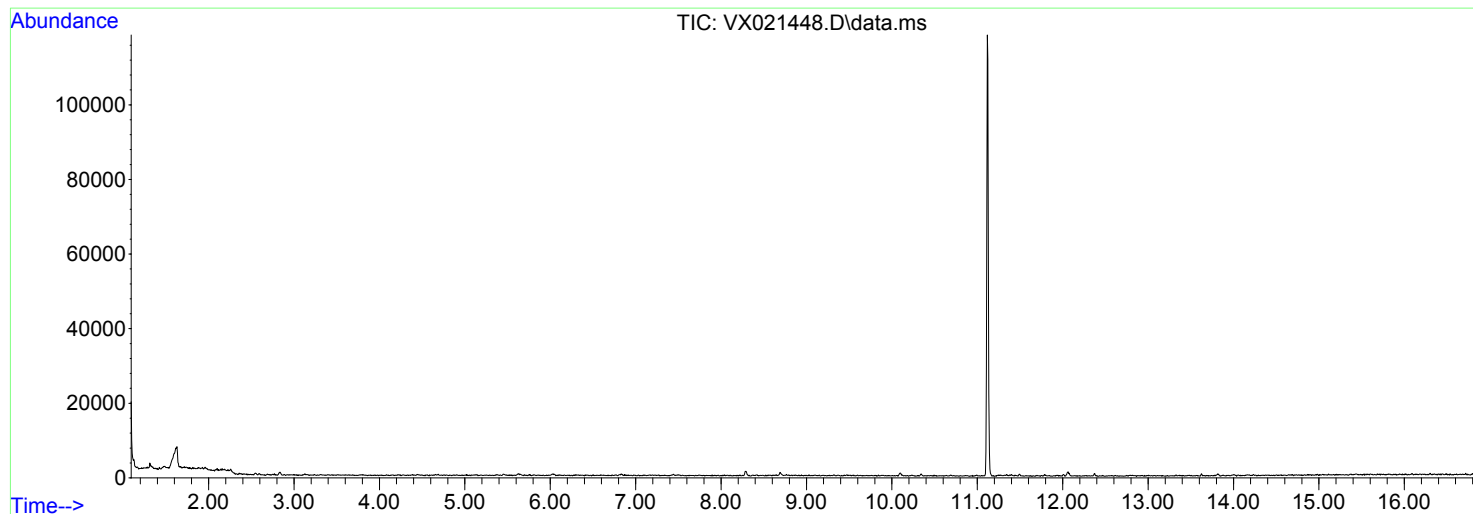

Spectrum Information: Average of 11.112 to 11.124 min.

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.2	4538	PASS
75	95	30	60	56.0	11473	PASS
95	95	100	100	100.0	20484	PASS
96	95	5	9	7.1	1457	PASS
173	174	0.00	2	1.0	137	PASS
174	95	50	100	68.5	14024	PASS
175	174	5	9	8.1	1142	PASS
176	174	95	101	96.9	13587	PASS
177	176	5	9	7.4	1011	PASS