

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032423\
 Data File : VX034724.D
 Acq On : 24 Mar 2023 16:29
 Operator : JC/MD
 Sample : 02052-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 AUD-1700

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
 Title : SW846 8260

Signal : TIC: VX034724.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.550	232	240	253	rBV2	9719	27750	1.62%	0.295%
2	4.562	558	570	581	rBV2	5075	18619	1.09%	0.198%
3	5.385	693	705	721	rBV	193232	563127	32.82%	5.993%
4	5.550	721	732	750	rVB	339813	980980	57.17%	10.439%
5	5.952	788	798	817	rBV	227034	612049	35.67%	6.513%
6	6.763	921	931	949	rBV	527372	1290819	75.23%	13.736%
7	8.647	1233	1240	1248	rBV	1097399	1715879	100.00%	18.260%
8	8.720	1248	1252	1261	rVB	11824	22756	1.33%	0.242%
9	10.055	1465	1471	1481	rBV	1062868	1478455	86.16%	15.733%
10	11.079	1634	1639	1652	rBV	906986	1148655	66.94%	12.223%
11	12.024	1788	1794	1802	rBV	1029500	1351502	78.76%	14.382%
12	13.256	1985	1996	2015	rVB5	23544	111379	6.49%	1.185%
13	13.500	2020	2036	2041	rBV10	12848	50533	2.95%	0.538%
14	15.347	2330	2339	2343	rBV10	7741	24658	1.44%	0.262%




Sum of corrected areas: 9397161

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032423\
Data File : VX034724.D
Acq On : 24 Mar 2023 16:29
Operator : JC/MD
Sample : 02052-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AUD-1700

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

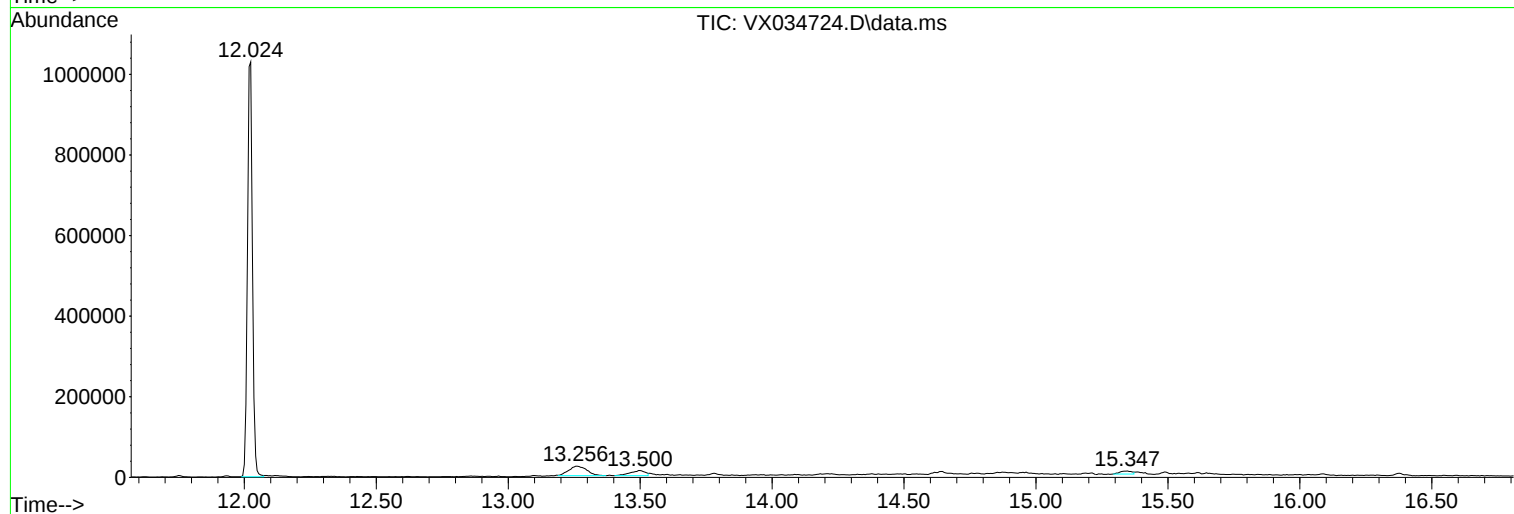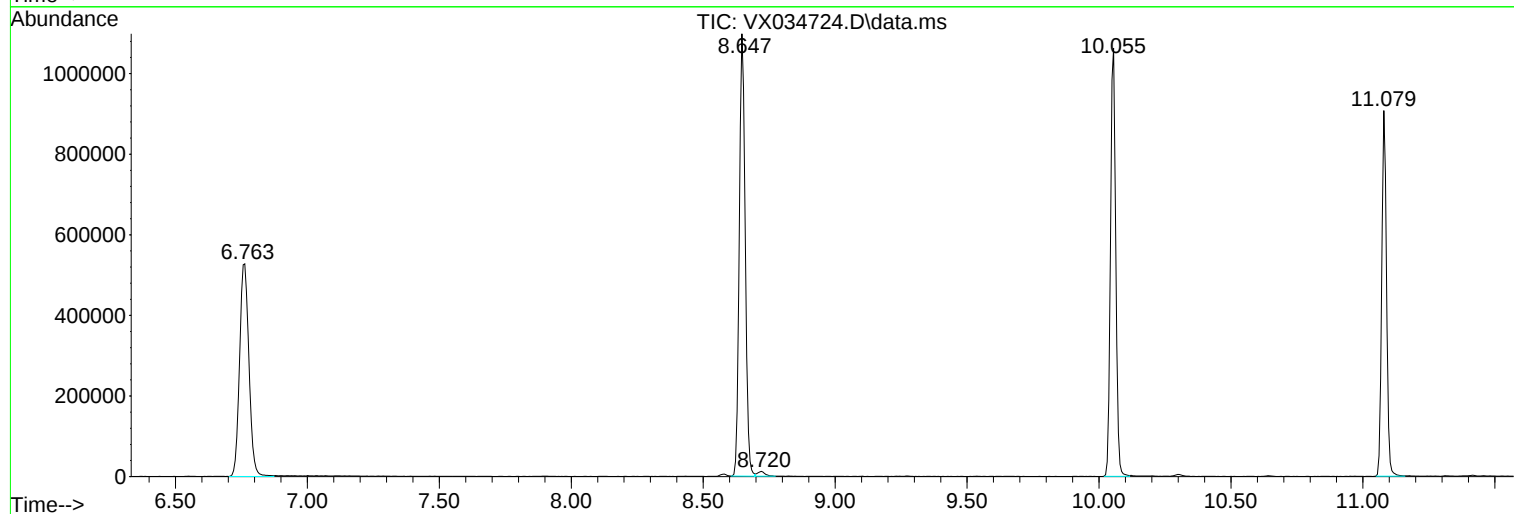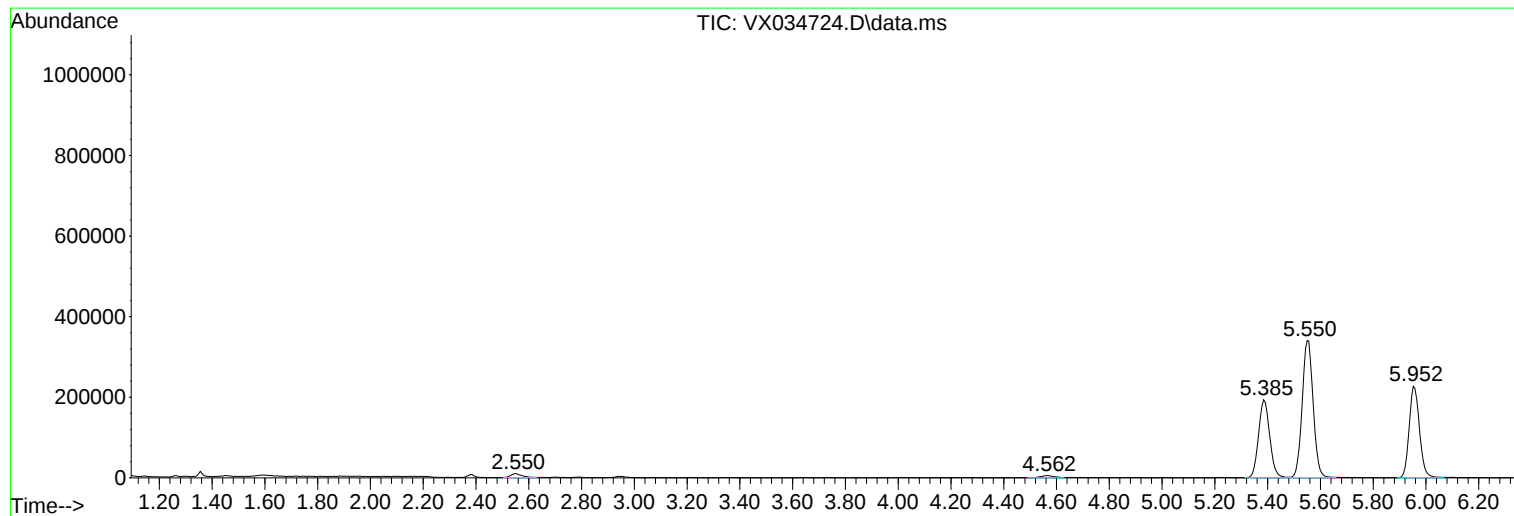

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032423\
Data File : VX034724.D
Acq On : 24 Mar 2023 16:29
Operator : JC/MD
Sample : 02052-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AUD-1700

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032423\
Data File : VX034724.D
Acq On : 24 Mar 2023 16:29
Operator : JC/MD
Sample : 02052-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AUD-1700

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------