

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032423\
Data File : VX034725.D
Acq On : 24 Mar 2023 16:52
Operator : JC/MD
Sample : 02056-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
025-OUTFALL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M

Title : SW846 8260

Signal : TIC: VX034725.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.380	206	212	225	rBV	17476	32505	1.96%	0.350%
2	5.385	692	705	721	rBV	183572	541326	32.69%	5.833%
3	5.550	721	732	748	rVB	335625	947017	57.19%	10.205%
4	5.952	787	798	818	rBV	218249	591588	35.73%	6.375%
5	6.763	921	931	946	rBV	511344	1230657	74.32%	13.261%
6	8.647	1234	1240	1249	rBV	1057249	1655879	100.00%	17.844%
7	10.055	1465	1471	1490	rBV	1040492	1432872	86.53%	15.440%
8	10.652	1564	1569	1580	rBV	288603	404020	24.40%	4.354%
9	11.079	1634	1639	1650	rBV	863259	1117218	67.47%	12.039%
10	11.756	1745	1750	1759	rBV2	9617	17986	1.09%	0.194%
11	12.018	1788	1793	1803	rBV	1017234	1308940	79.05%	14.105%




Sum of corrected areas: 9280008

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032423\
Data File : VX034725.D
Acq On : 24 Mar 2023 16:52
Operator : JC/MD
Sample : 02056-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
025-OUTFALL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

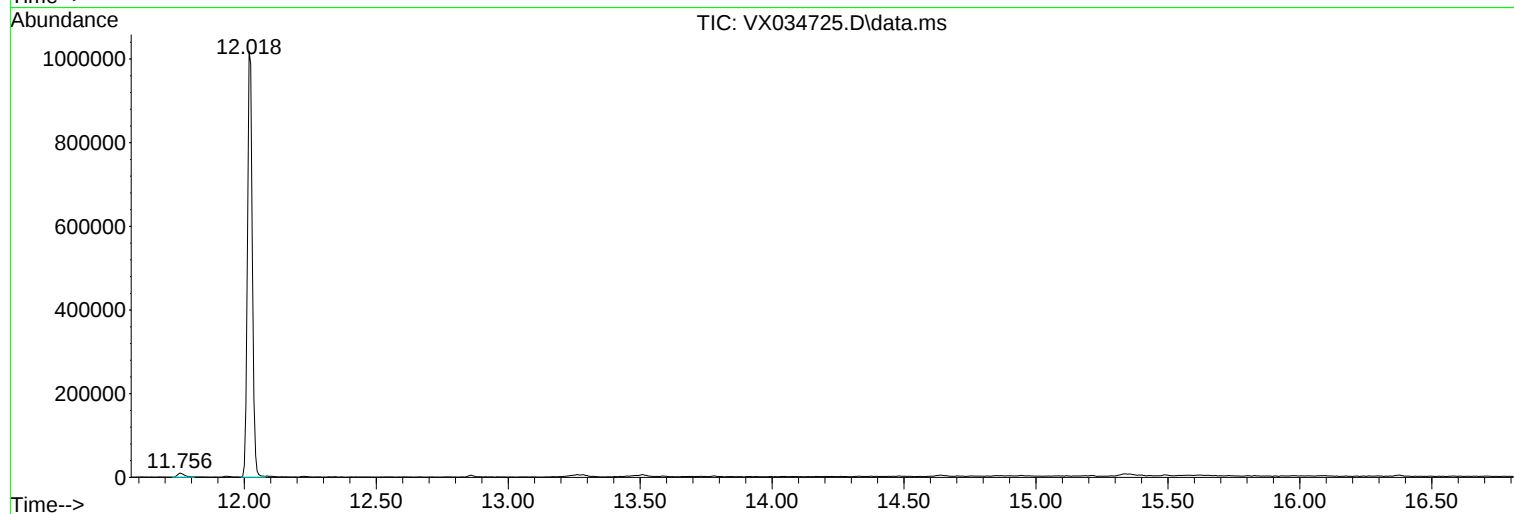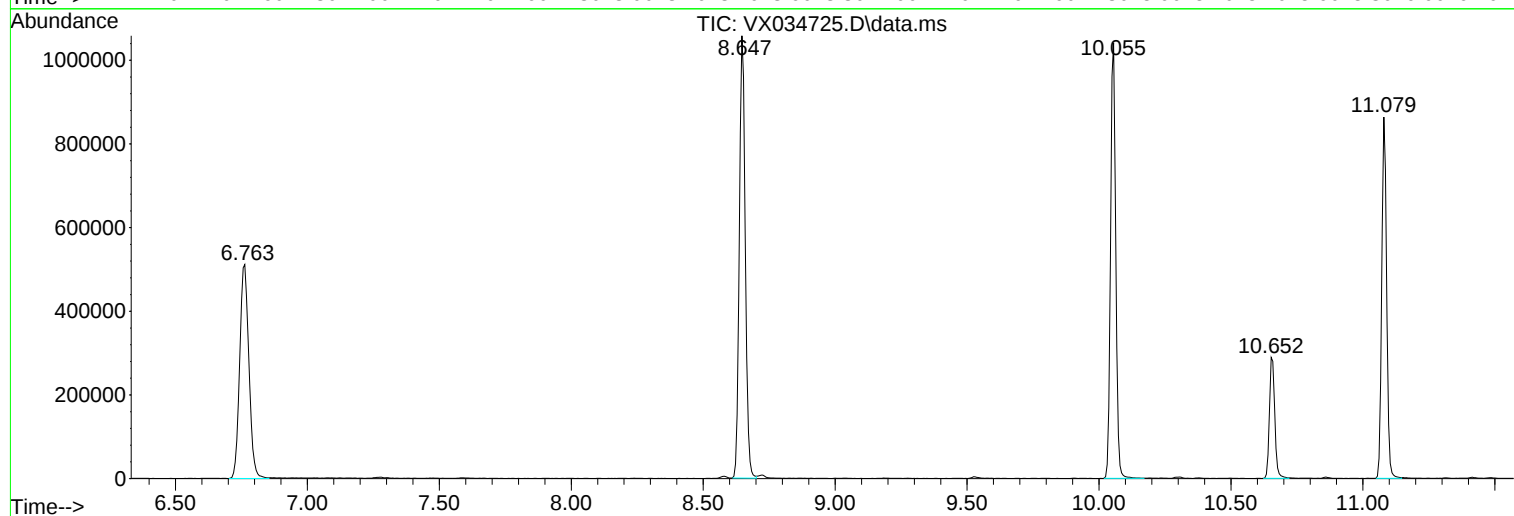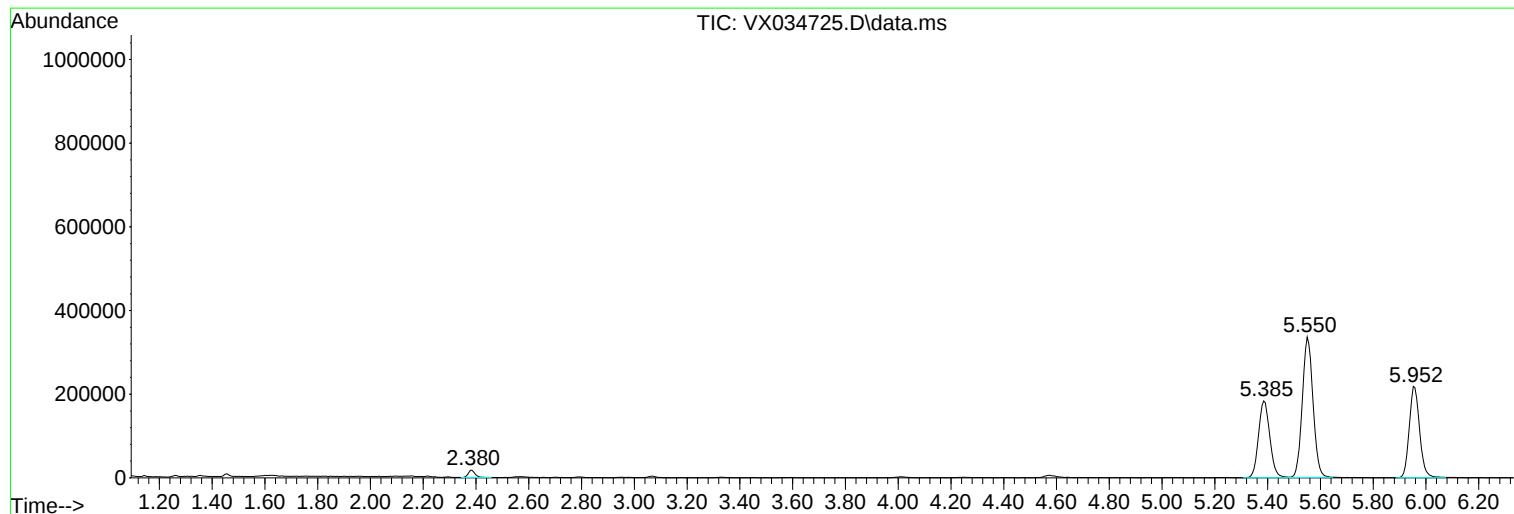

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032423\
Data File : VX034725.D
Acq On : 24 Mar 2023 16:52
Operator : JC/MD
Sample : 02056-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
025-OUTFALL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032423\
Data File : VX034725.D
Acq On : 24 Mar 2023 16:52
Operator : JC/MD
Sample : 02056-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
025-OUTFALL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc