

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032423\
 Data File : VX034733.D
 Acq On : 24 Mar 2023 19:57
 Operator : JC/MD
 Sample : 02080-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 T-5

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
 Title : SW846 8260

Signal : TIC: VX034733.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.111	320	332	349	rBV	983139	2267608	100.00%	19.313%
2	5.385	692	705	720	rBV	198688	575306	25.37%	4.900%
3	5.550	722	732	749	rVB	348606	996447	43.94%	8.487%
4	5.952	788	798	817	rBV	231698	615624	27.15%	5.243%
5	6.324	848	859	872	rBV2	20951	61387	2.71%	0.523%
6	6.763	920	931	950	rBV	540685	1308627	57.71%	11.146%
7	8.647	1233	1240	1250	rBV	1118612	1762495	77.72%	15.011%
8	10.055	1465	1471	1483	rBV	1086127	1521247	67.09%	12.956%
9	11.079	1634	1639	1654	rBV	912668	1177102	51.91%	10.025%
10	12.024	1788	1794	1805	rBV	1087337	1393630	61.46%	11.870%
11	13.140	1972	1977	1987	rBV2	41724	61780	2.72%	0.526%




Sum of corrected areas: 11741253

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032423\
Data File : VX034733.D
Acq On : 24 Mar 2023 19:57
Operator : JC/MD
Sample : 02080-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
T-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

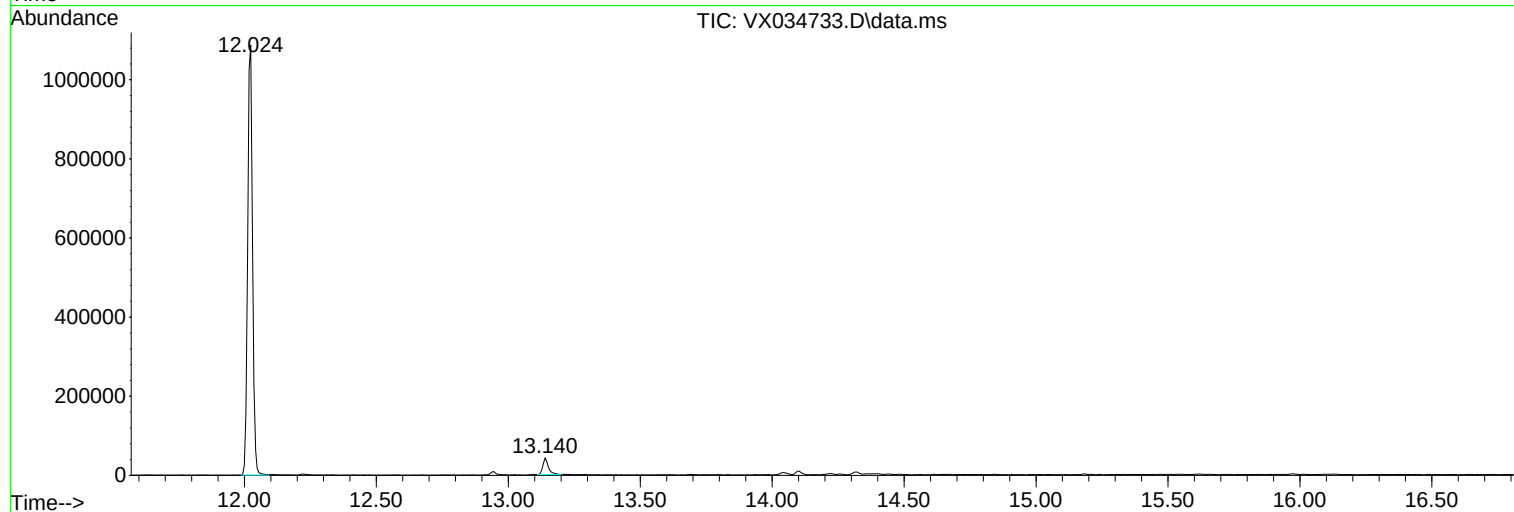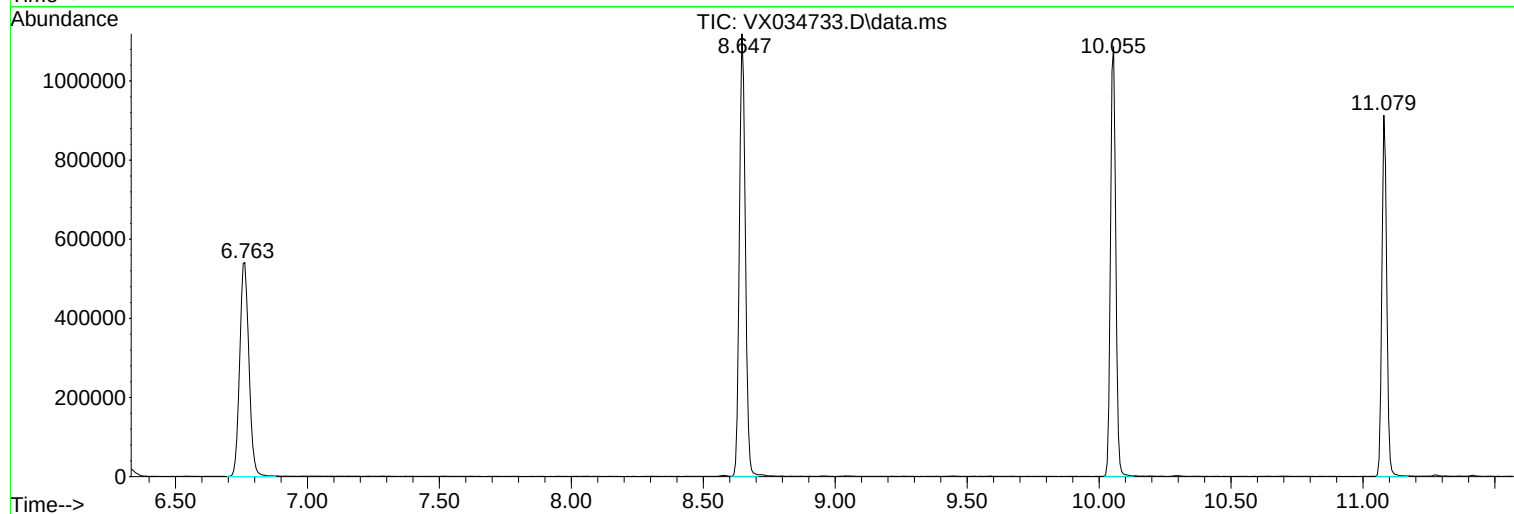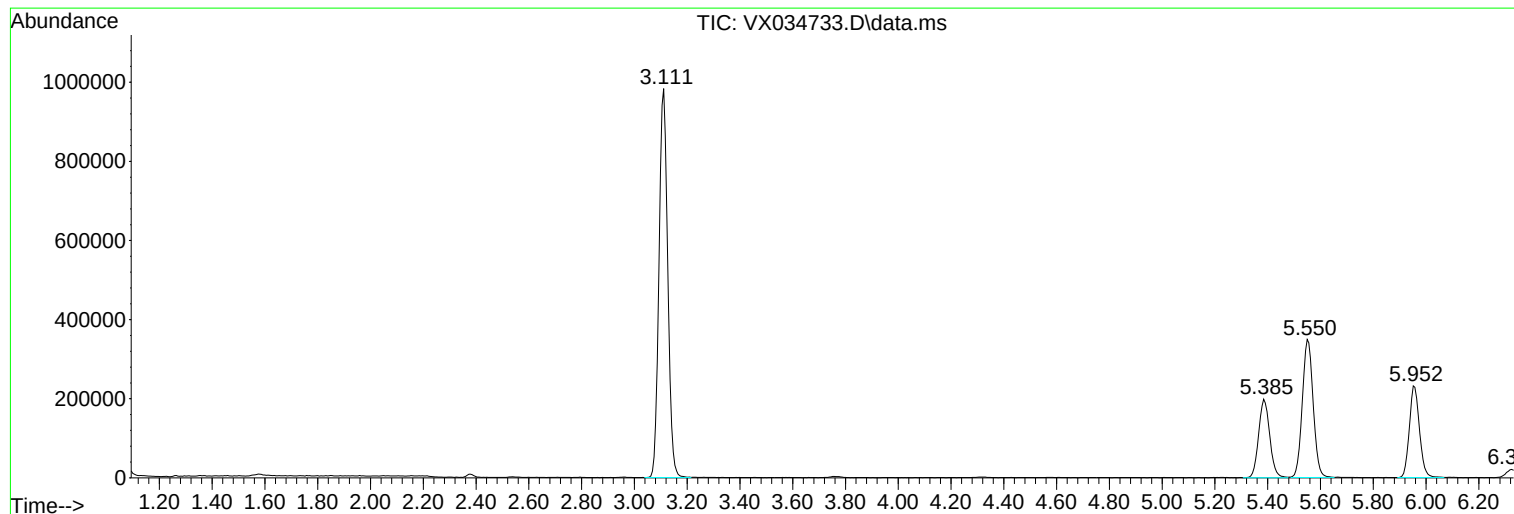

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032423\
Data File : VX034733.D
Acq On : 24 Mar 2023 19:57
Operator : JC/MD
Sample : 02080-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
T-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032423\
Data File : VX034733.D
Acq On : 24 Mar 2023 19:57
Operator : JC/MD
Sample : 02080-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
T-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------