

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032423\
 Data File : VX034734.D
 Acq On : 24 Mar 2023 20:21
 Operator : JC/MD
 Sample : 02080-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 T-6

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M

Title : SW846 8260

Signal : TIC: VX034734.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.111	321	332	344	rBV	84592	189123	11.23%	2.055%
2	4.312	519	529	541	rBV3	14552	45404	2.70%	0.493%
3	5.385	692	705	719	rBV	188944	545968	32.43%	5.933%
4	5.550	721	732	749	rVV	332801	952877	56.60%	10.355%
5	5.952	788	798	821	rBV	216972	591572	35.14%	6.429%
6	6.763	920	931	957	rBV	515684	1255642	74.59%	13.645%
7	8.647	1233	1240	1251	rBV	1078377	1683485	100.00%	18.295%
8	10.055	1465	1471	1490	rBV	1059056	1456294	86.50%	15.826%
9	11.079	1633	1639	1658	rBV	875132	1126631	66.92%	12.243%
10	12.018	1788	1793	1807	rBV	1020877	1315950	78.17%	14.301%
11	13.140	1970	1977	1988	rBV	23935	38959	2.31%	0.423%




Sum of corrected areas: 9201905

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032423\
Data File : VX034734.D
Acq On : 24 Mar 2023 20:21
Operator : JC/MD
Sample : 02080-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
T-6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

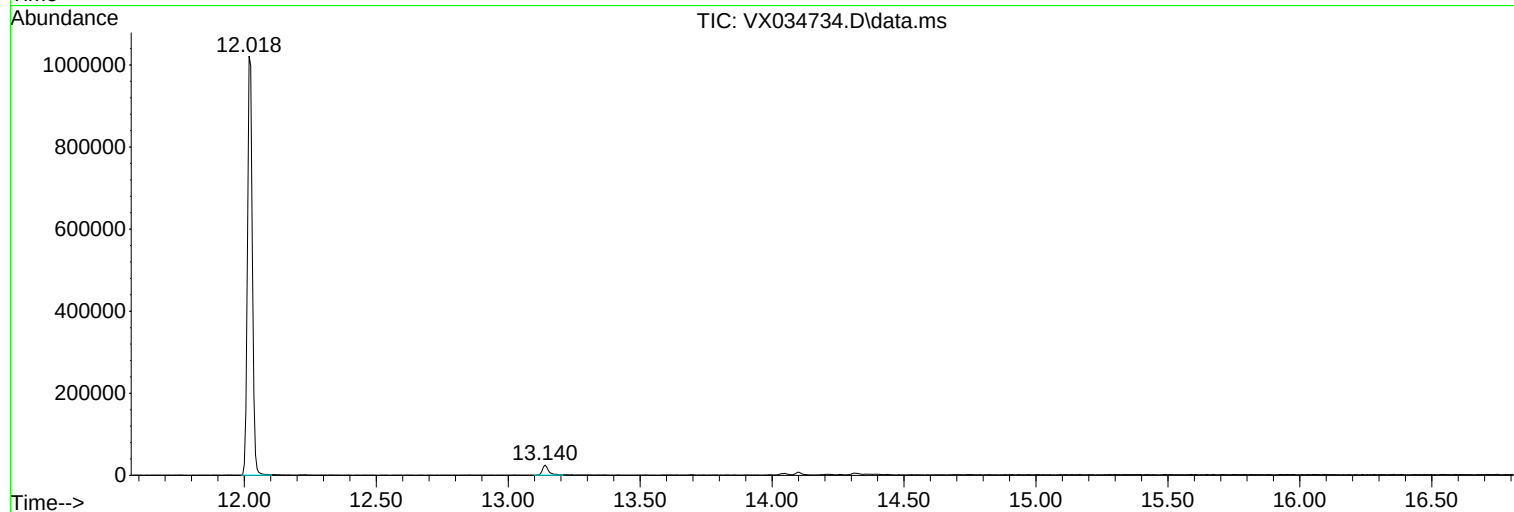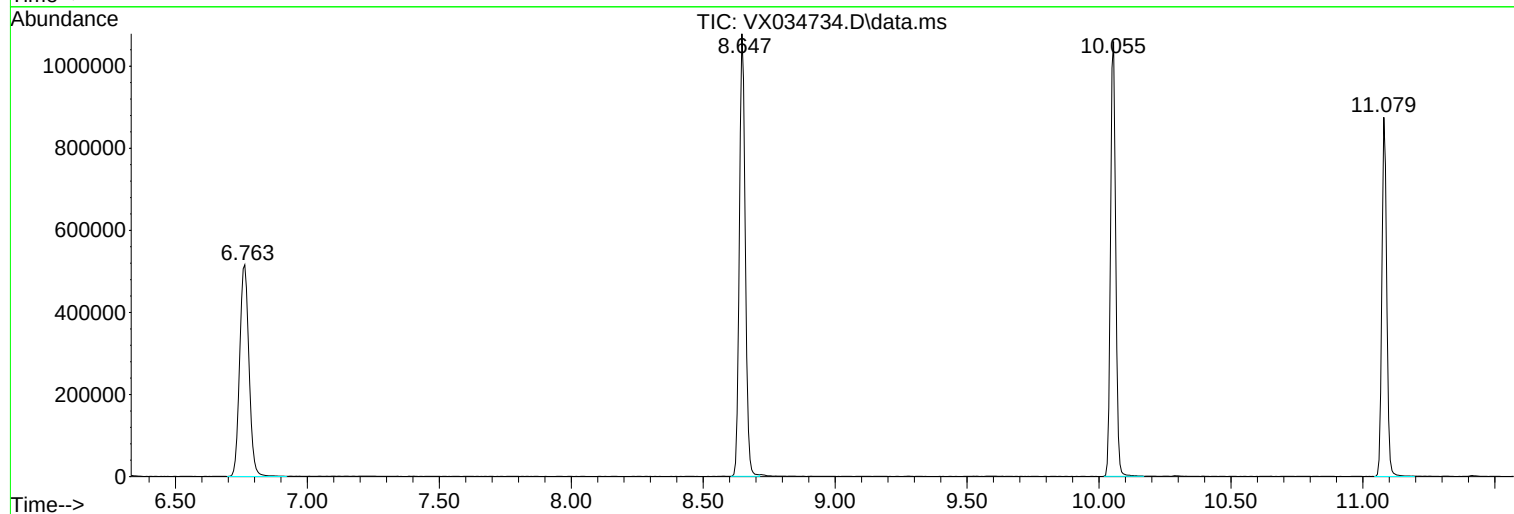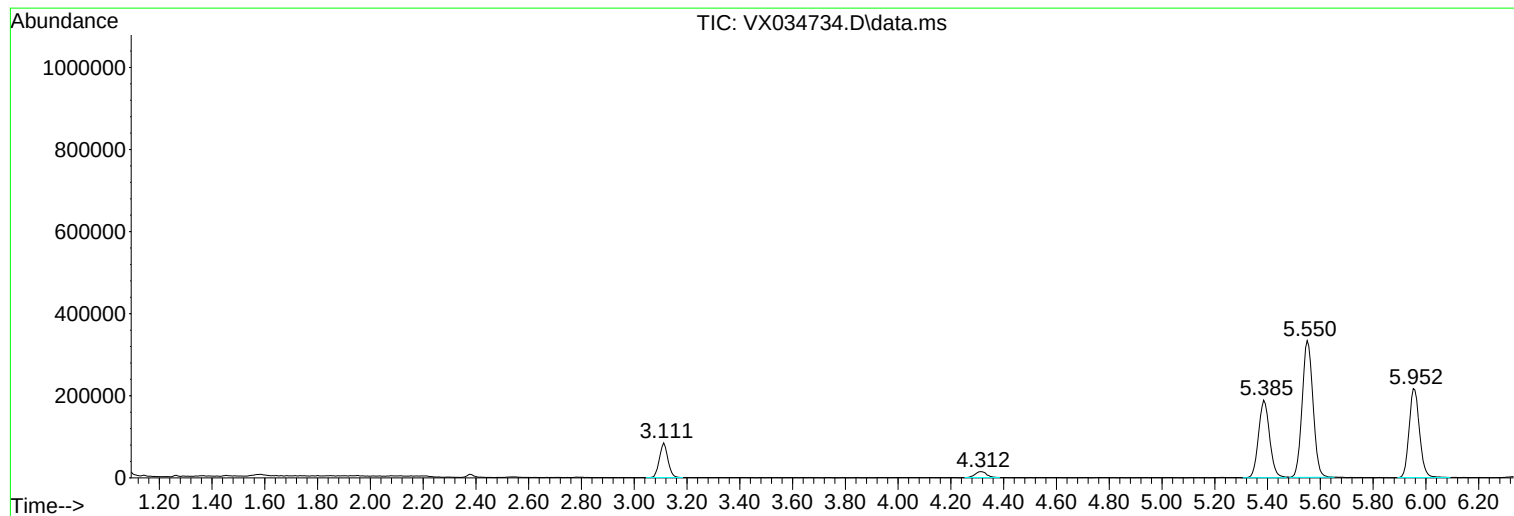

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032423\
Data File : VX034734.D
Acq On : 24 Mar 2023 20:21
Operator : JC/MD
Sample : 02080-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
T-6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032423\
Data File : VX034734.D
Acq On : 24 Mar 2023 20:21
Operator : JC/MD
Sample : 02080-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
T-6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------