

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032425\
 Data File : VX045424.D
 Acq On : 24 Mar 2025 18:46
 Operator : JC/MD
 Sample : Q1608-24
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RW8-MW01S-20250319

Quant Time: Mar 25 01:39:27 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:45:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.544	168	67003	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	132767	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	123522	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	50743	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	61799	57.985	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	115.960%
35) Dibromofluoromethane	5.385	113	46424	52.292	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	104.580%
50) Toluene-d8	8.647	98	162777	50.575	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	101.160%
62) 4-Bromofluorobenzene	11.079	95	56684	53.149	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	106.300%
Target Compounds						
16) Acetone	2.386	43	862	1.743	ug/l	100
44) Trichloroethene	7.135	130	1532	1.697	ug/l	74

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032425\
Data File : VX045424.D
Acq On : 24 Mar 2025 18:46
Operator : JC/MD
Sample : Q1608-24
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RW8-MW01S-20250319

Quant Time: Mar 25 01:39:27 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 28 06:45:16 2025
Response via : Initial Calibration



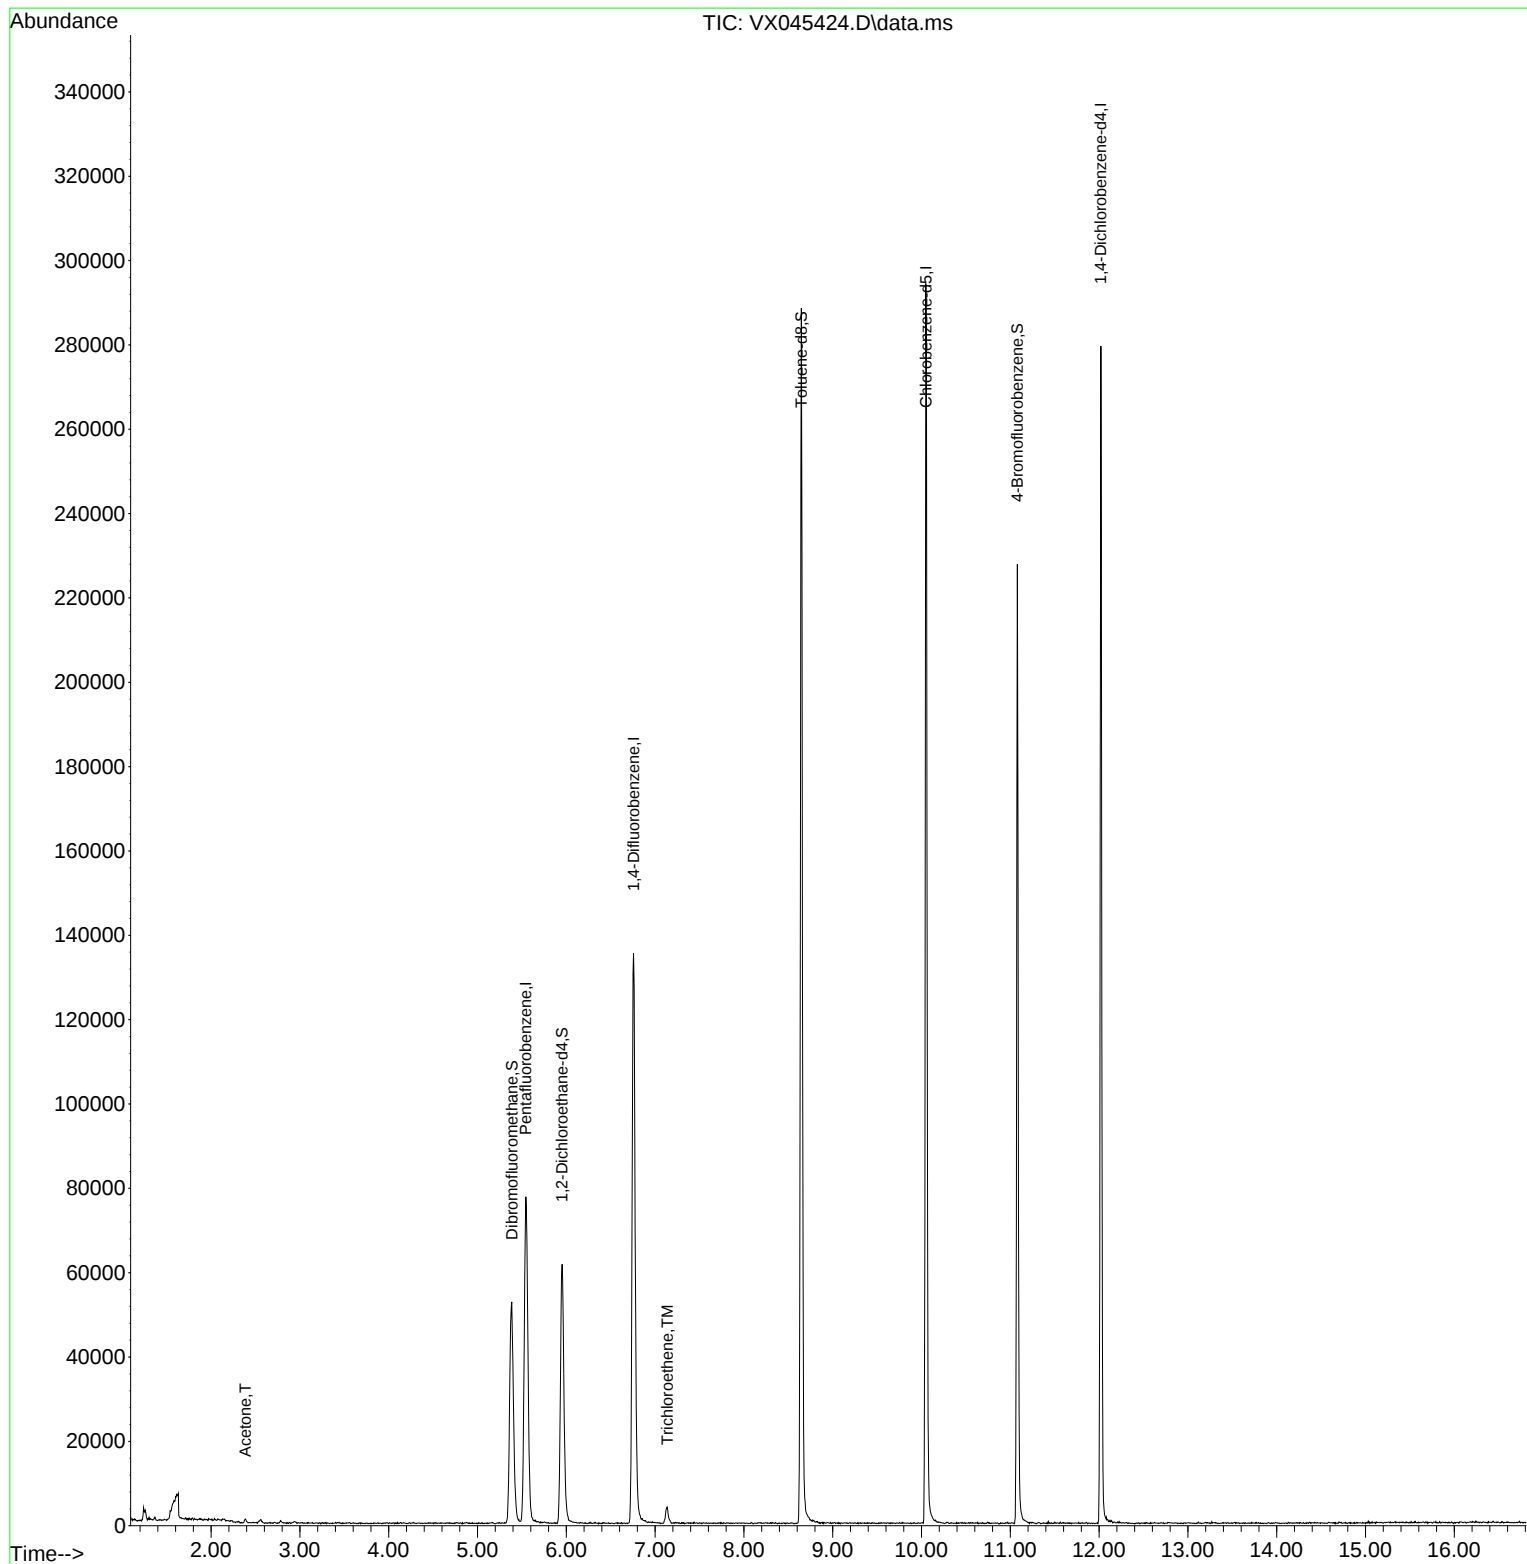




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.006 min
Lab File: VX045424.D
Acq: 24 Mar 2025 18:46




Instrument :
MSVOA_X
ClientSampleId :
RW8-MW01S-20250319

Tgt Ion:168 Resp: 67003
Ion Ratio Lower Upper
168 100
99 68.4 48.2 72.4

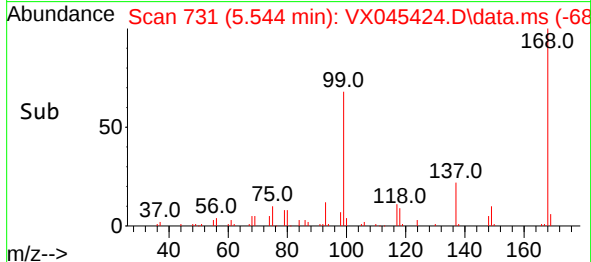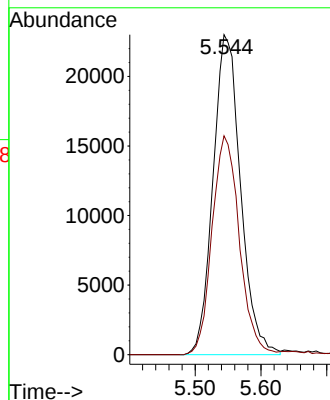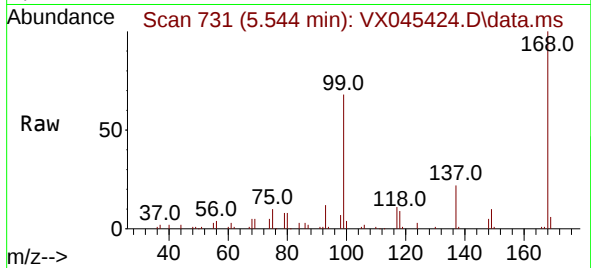

#16
Acetone
Concen: 1.743 ug/l
RT: 2.386 min Scan# 213
Delta R.T. 0.000 min
Lab File: VX045424.D
Acq: 24 Mar 2025 18:46

Tgt Ion: 43 Resp: 862
Ion Ratio Lower Upper
43 100
58 30.5 24.2 36.4

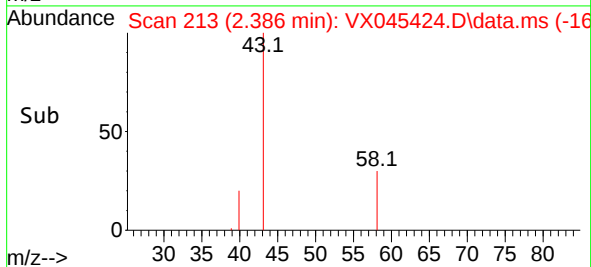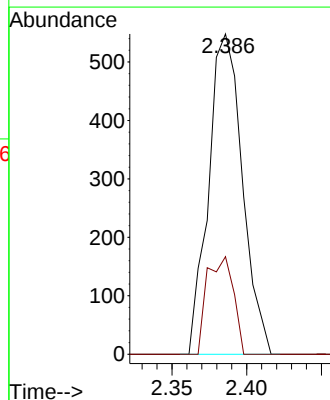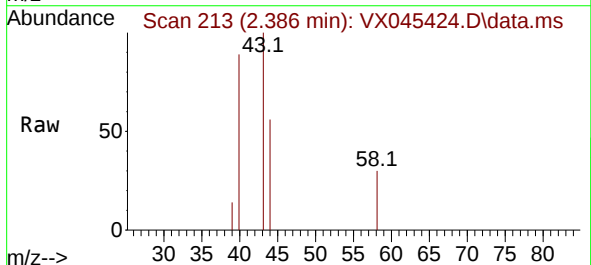



#33

1,2-Dichloroethane-d4

Concen: 57.985 ug/l

RT: 5.952 min Scan# 798

Delta R.T. 0.000 min

Lab File: VX045424.D

Acq: 24 Mar 2025 18:46

Instrument :

MSVOA_X

ClientSampleId :





RW8-MW01S-20250319

Tgt Ion: 65 Resp: 61799

Ion Ratio Lower Upper

65 100

67 49.7 0.0 106.2

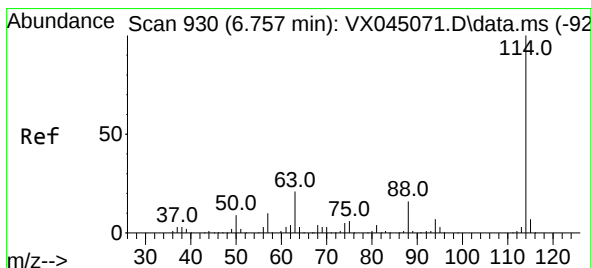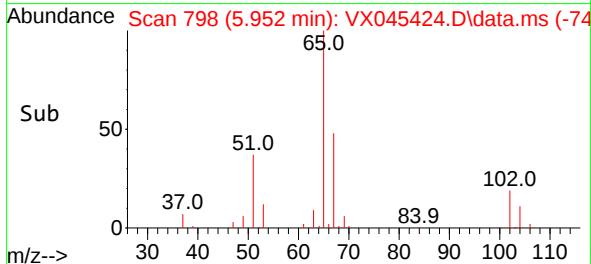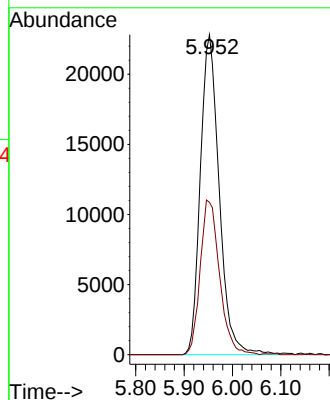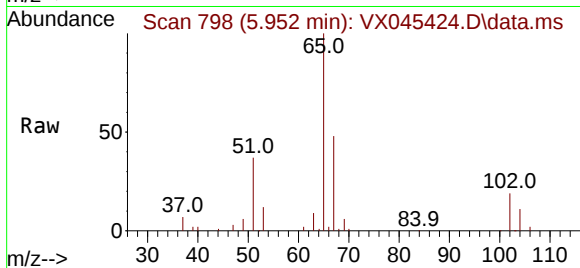

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. 0.000 min

Lab File: VX045424.D

Acq: 24 Mar 2025 18:46




Tgt Ion: 114 Resp: 132767

Ion Ratio Lower Upper

114 100

63 23.3 0.0 41.8

88 16.9 0.0 32.8


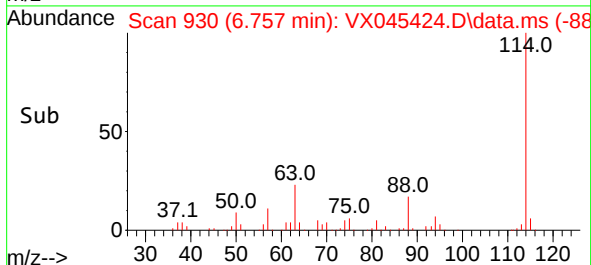
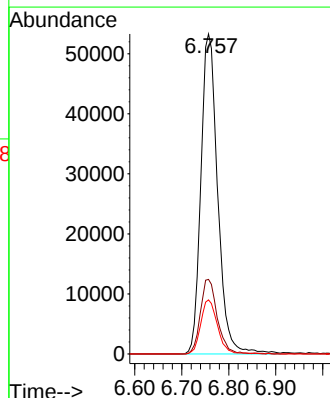
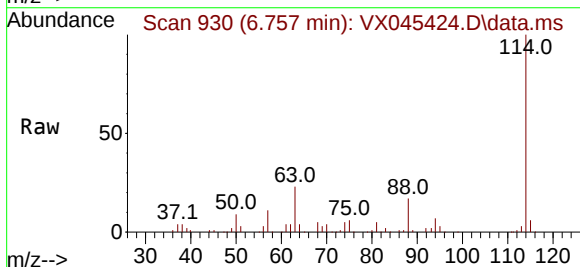




#35
Dibromofluoromethane
Concen: 52.292 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX045424.D
Acq: 24 Mar 2025 18:46




Instrument :
MSVOA_X
ClientSampleId :
RW8-MW01S-20250319


Tgt Ion:113 Resp: 46424
Ion Ratio Lower Upper
113 100
111 101.4 81.8 122.6
192 16.7 14.3 21.5

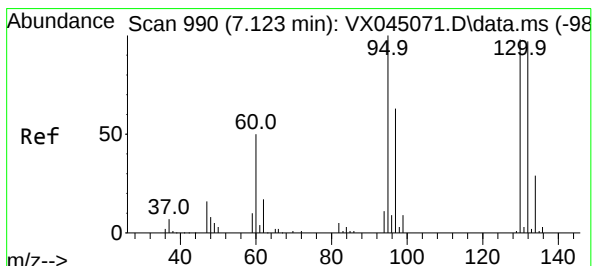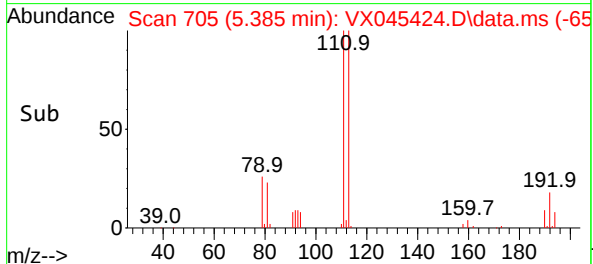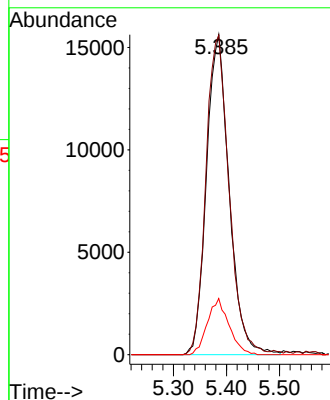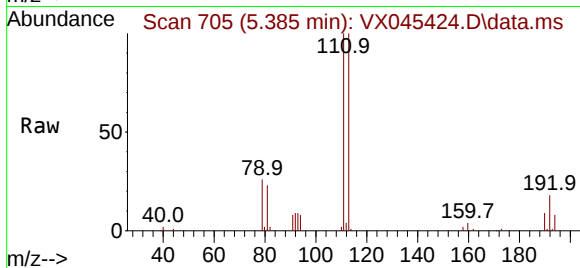

#44
Trichloroethene
Concen: 1.697 ug/l
RT: 7.135 min Scan# 992
Delta R.T. 0.012 min
Lab File: VX045424.D
Acq: 24 Mar 2025 18:46

Tgt Ion:130 Resp: 1532
Ion Ratio Lower Upper
130 100
95 128.8 0.0 205.0


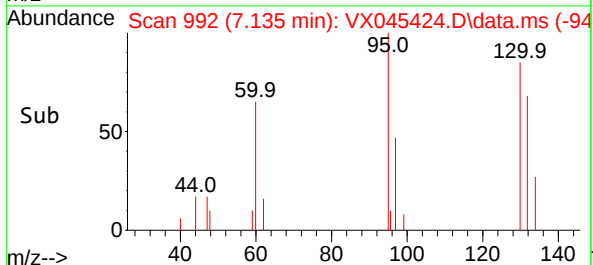
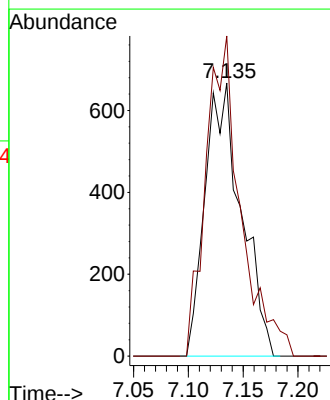
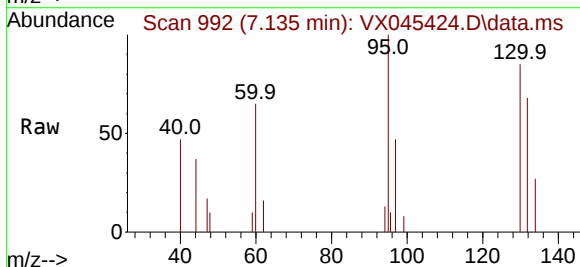


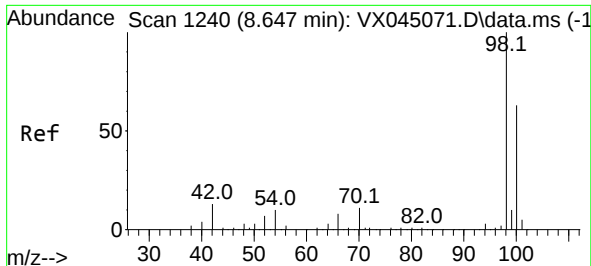

#50
Toluene-d8
Concen: 50.575 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX045424.D
Acq: 24 Mar 2025 18:46




Instrument :
MSVOA_X
ClientSampleId :
RW8-MW01S-20250319


Tgt Ion: 98 Resp: 162777
Ion Ratio Lower Upper
98 100
100 63.9 52.0 78.0

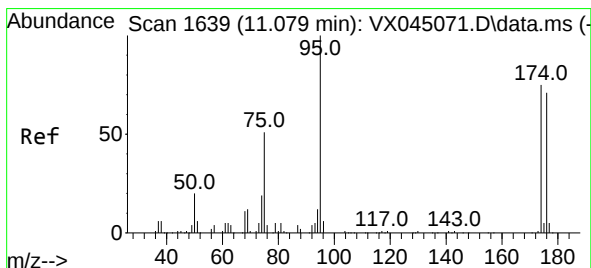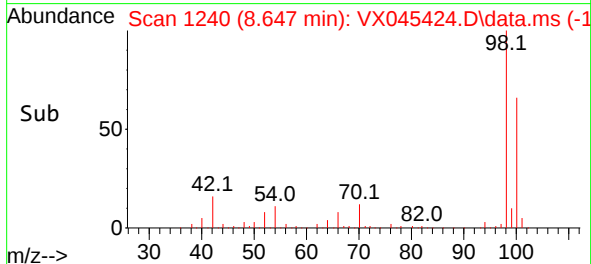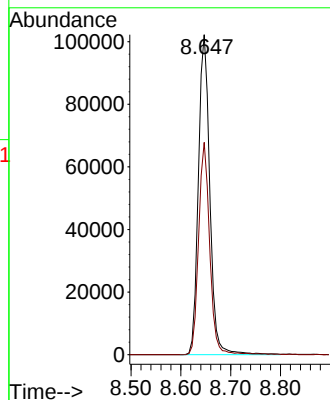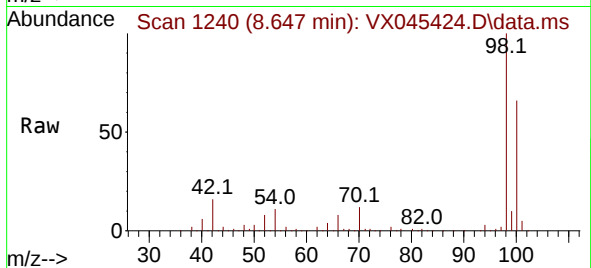

#62
4-Bromofluorobenzene
Concen: 53.149 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX045424.D
Acq: 24 Mar 2025 18:46

Tgt Ion: 95 Resp: 56684
Ion Ratio Lower Upper
95 100
174 70.1 0.0 148.2
176 66.9 0.0 141.4


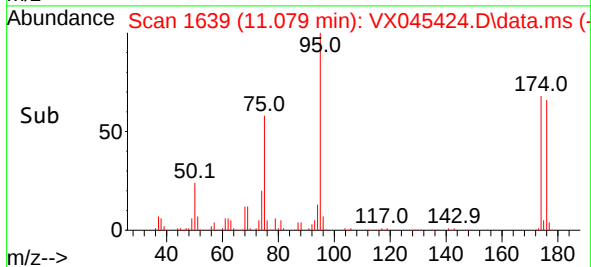
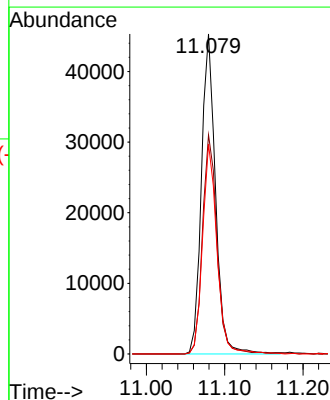
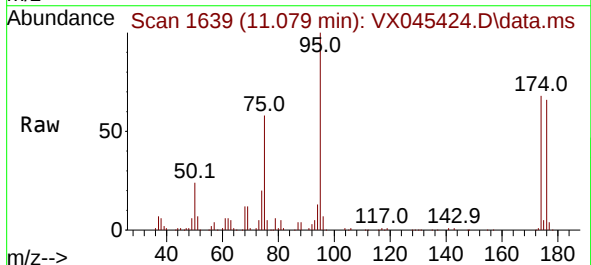


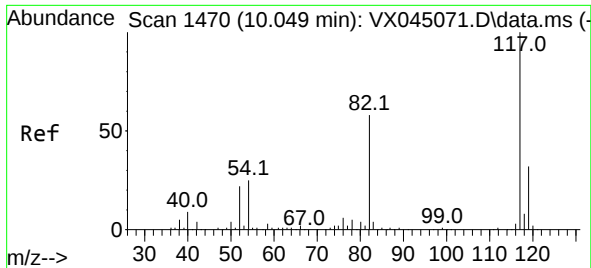

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. 0.000 min
Lab File: VX045424.D
Acq: 24 Mar 2025 18:46

Instrument :
MSVOA_X
ClientSampleId :
RW8-MW01S-20250319

Tgt Ion:117 Resp: 123522
Ion Ratio Lower Upper
117 100
82 61.7 46.3 69.5
119 32.3 25.7 38.5

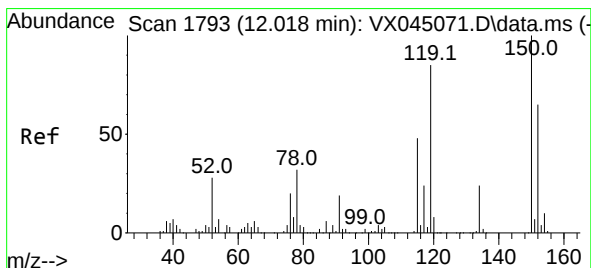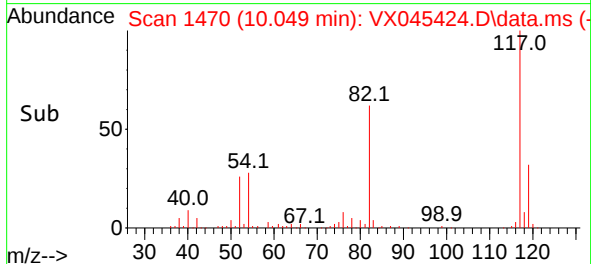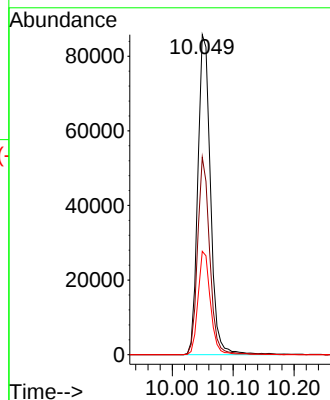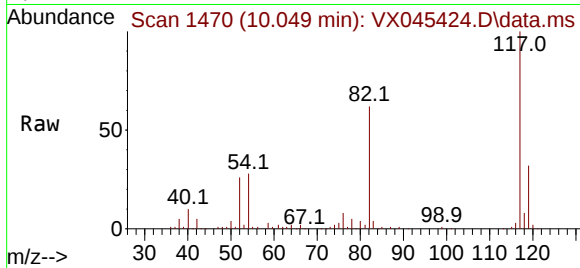

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. 0.000 min
Lab File: VX045424.D
Acq: 24 Mar 2025 18:46

Tgt Ion:152 Resp: 50743
Ion Ratio Lower Upper
152 100
115 63.4 44.2 132.6
150 160.4 0.0 349.0

