




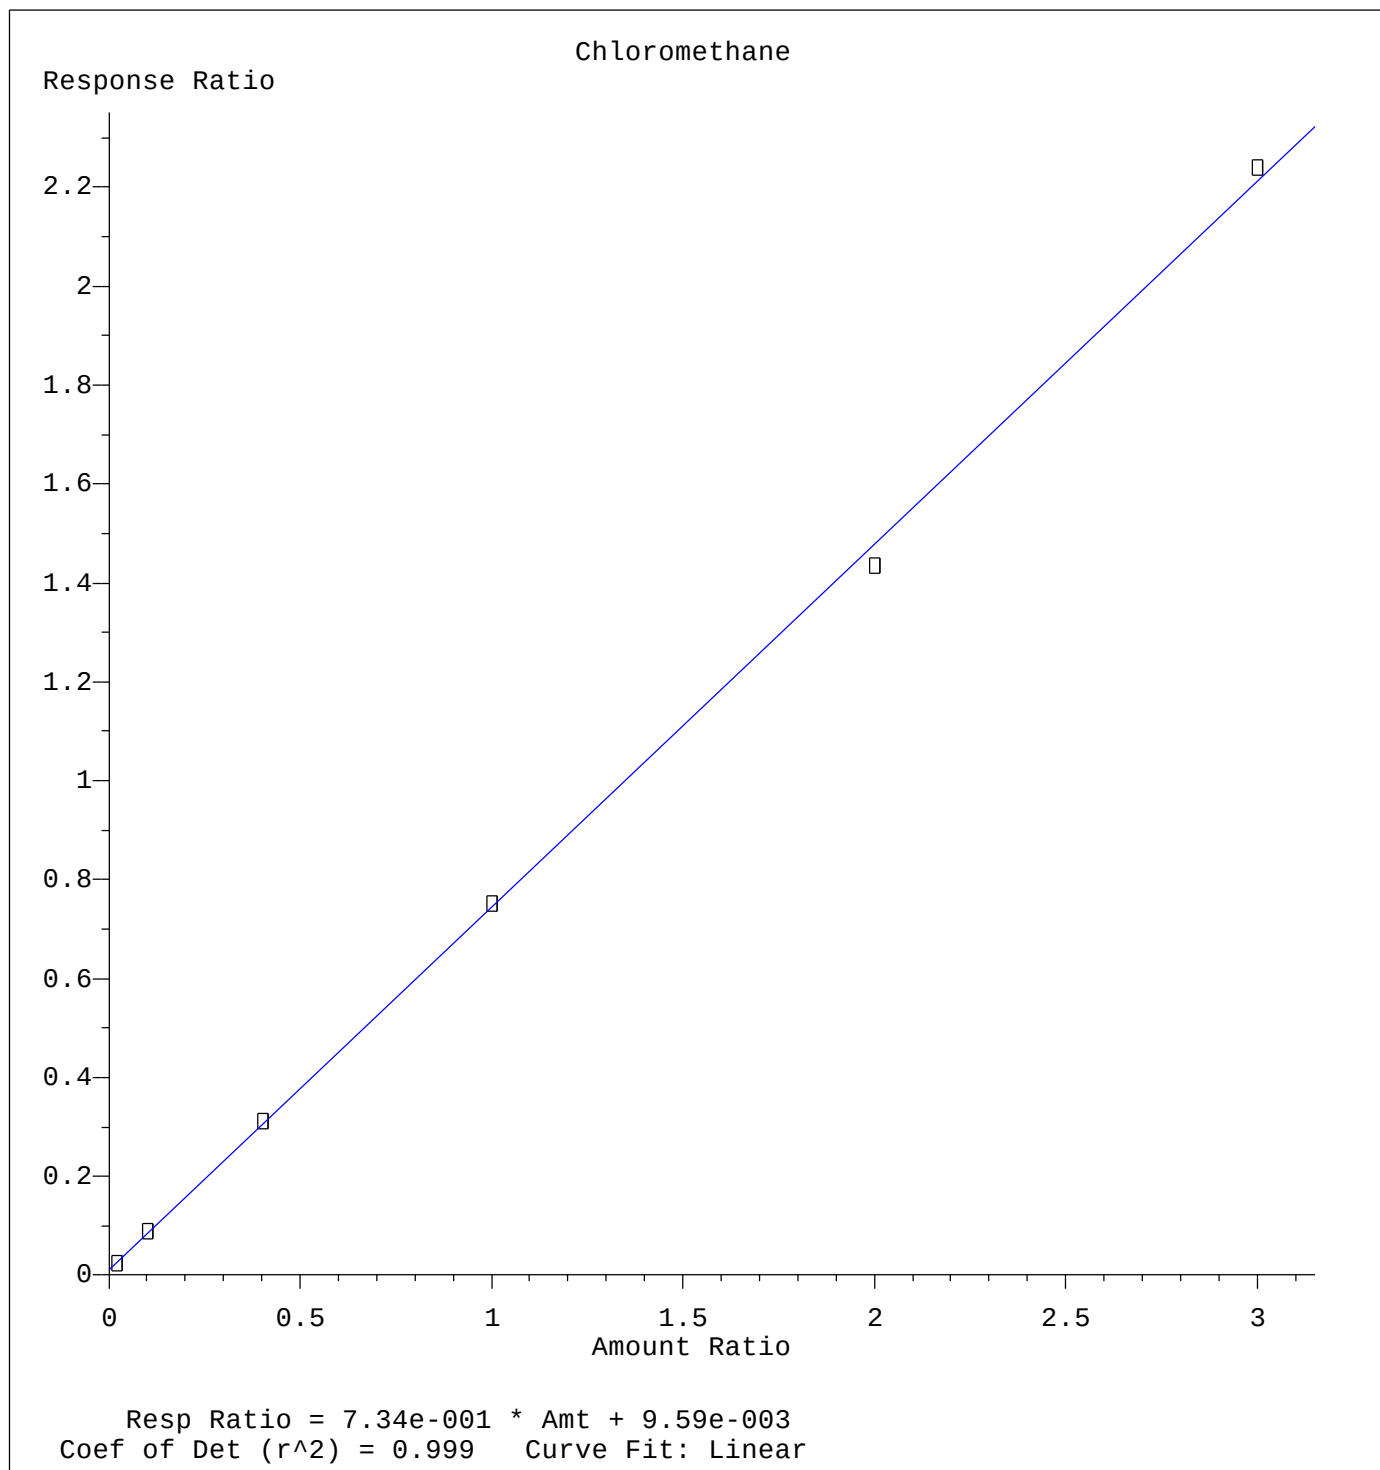


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X032519W.M
Calibration Table Last Updated: Tue Mar 26 07:57:20 2019

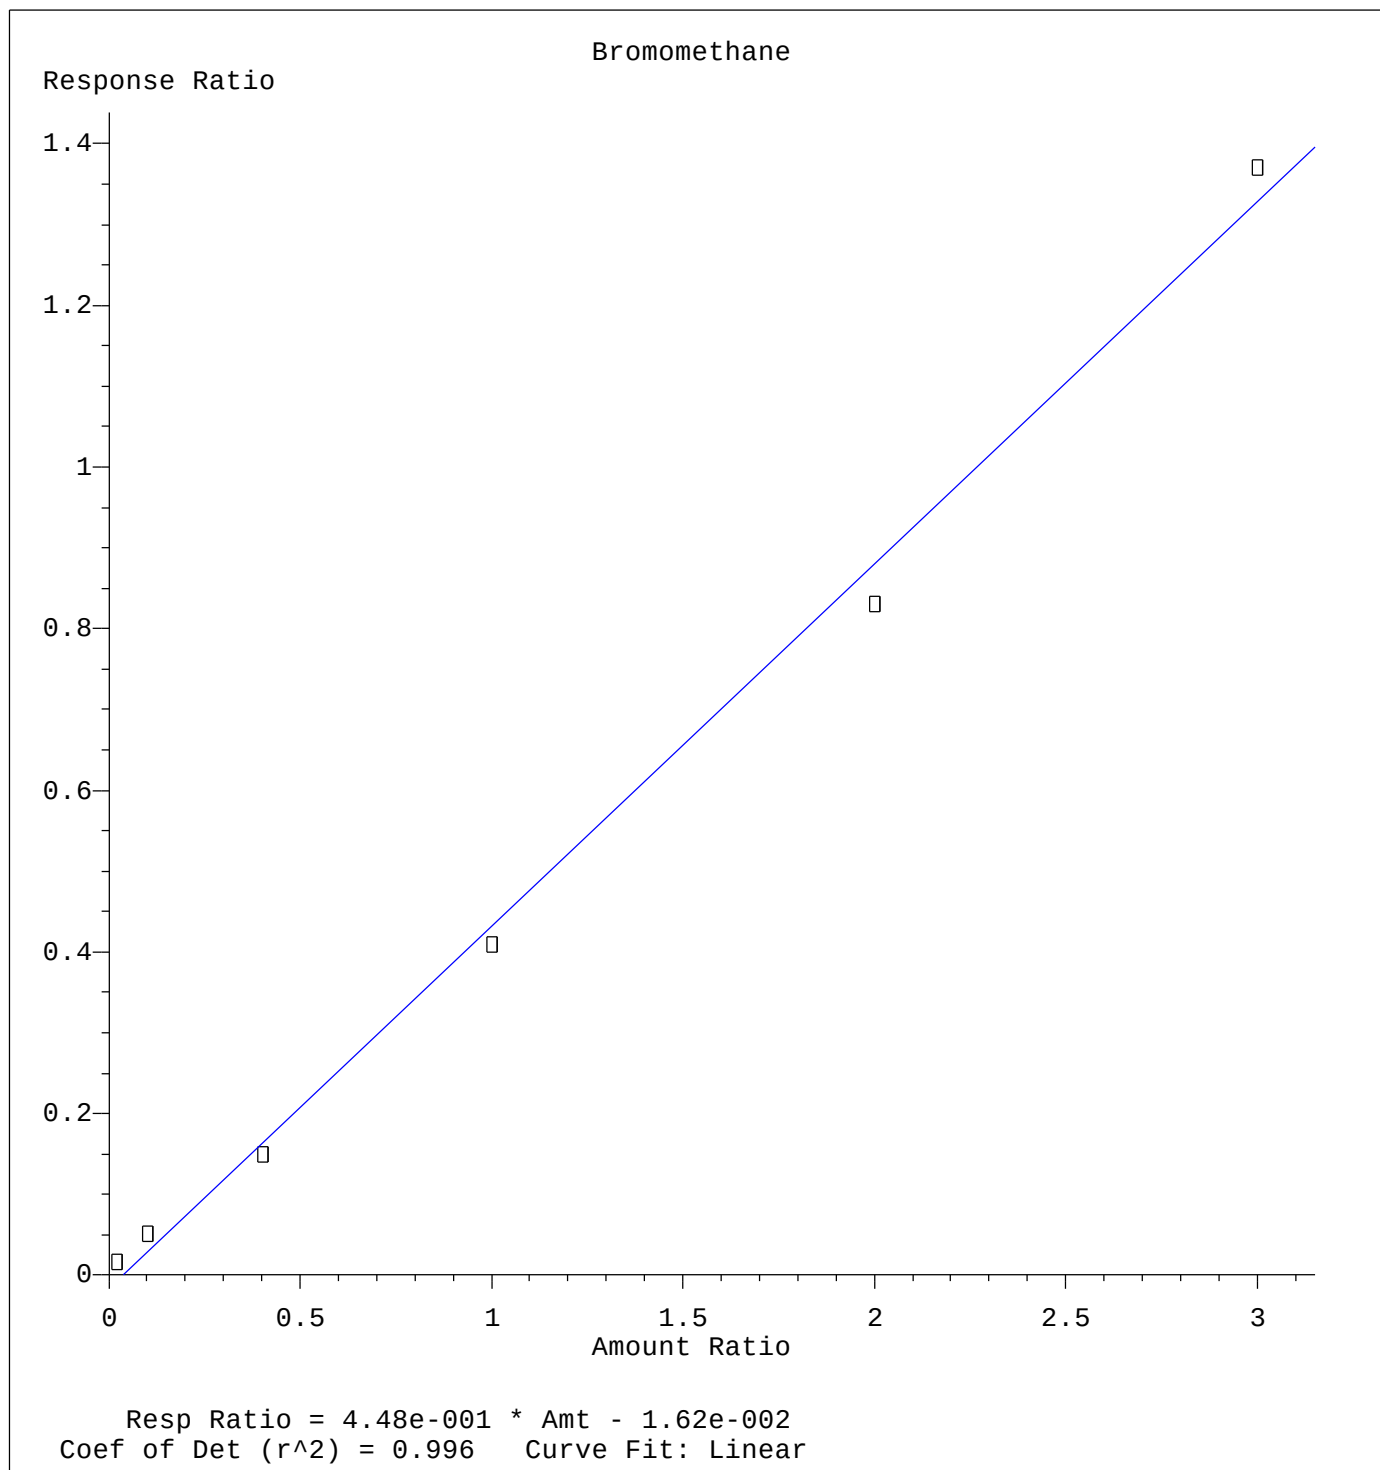

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X032519W.M
Calibration Table Last Updated: Tue Mar 26 07:57:20 2019

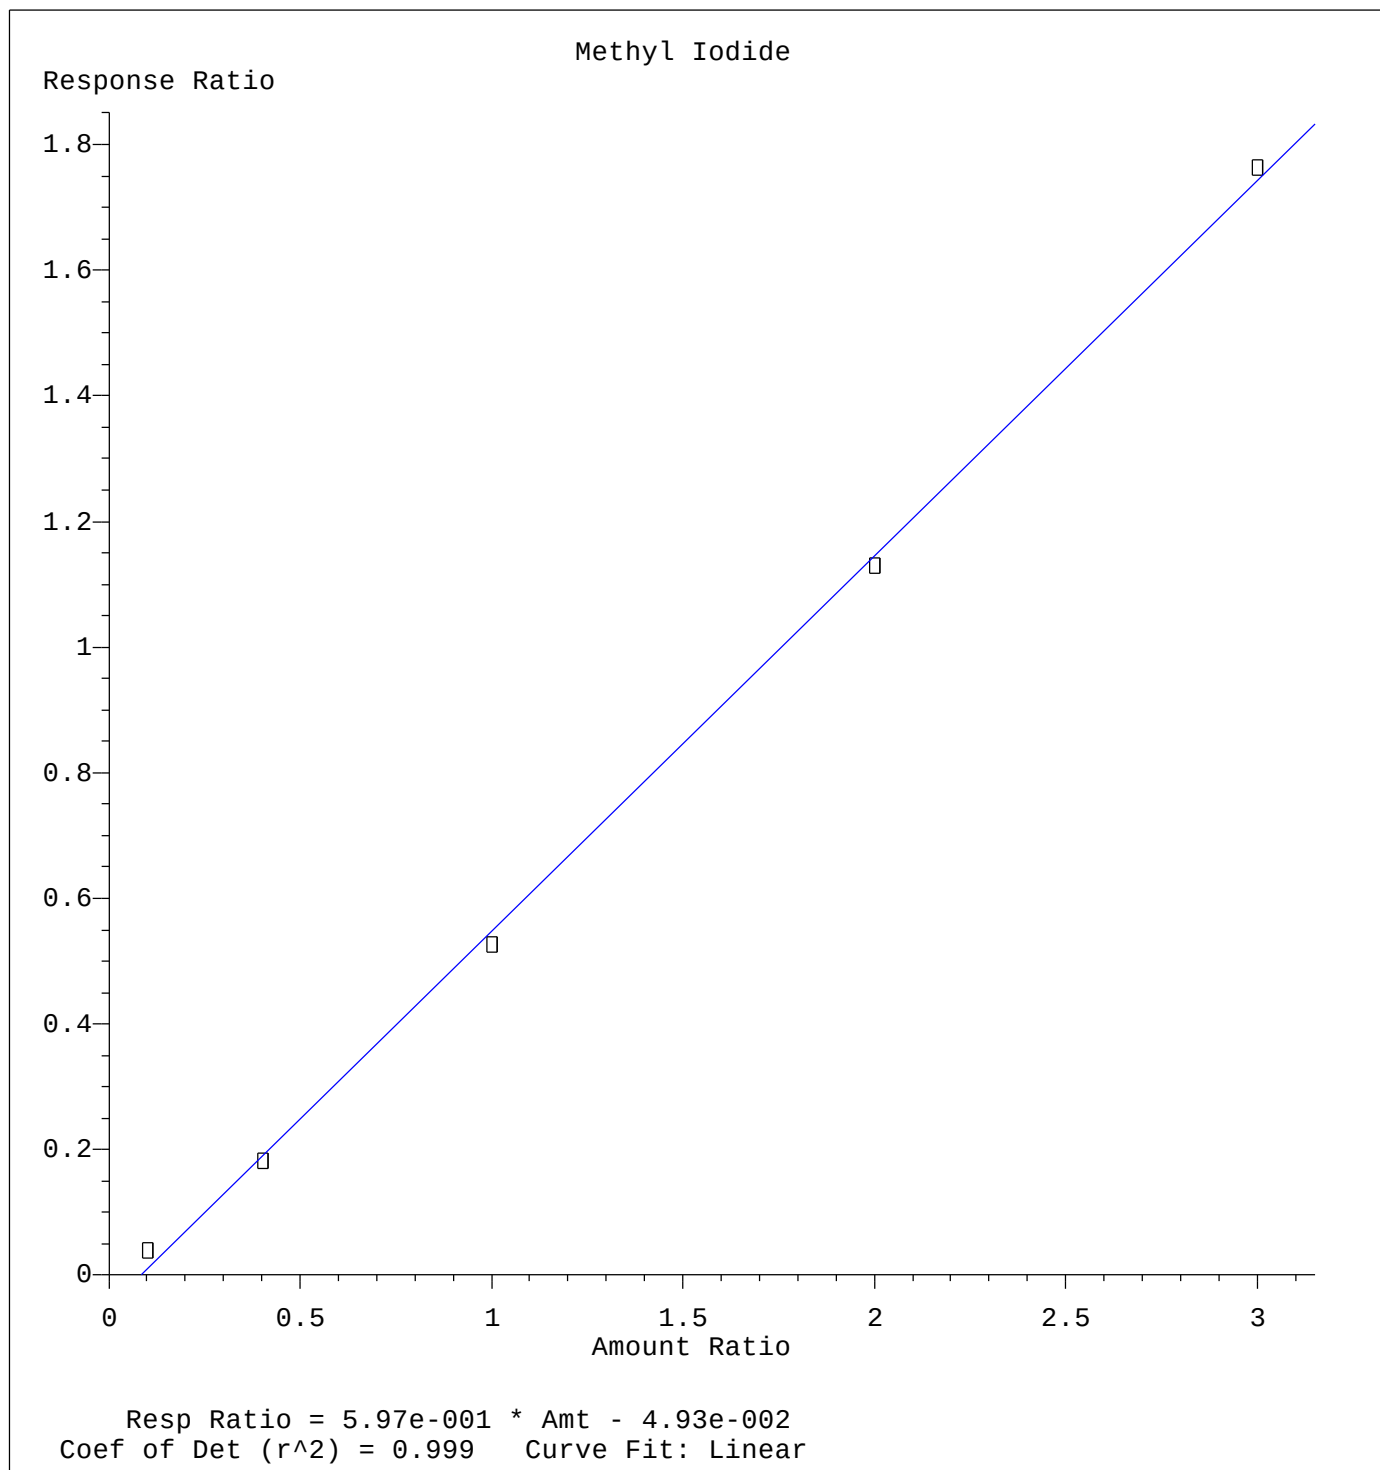


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X032519W.M
Calibration Table Last Updated: Tue Mar 26 07:57:20 2019

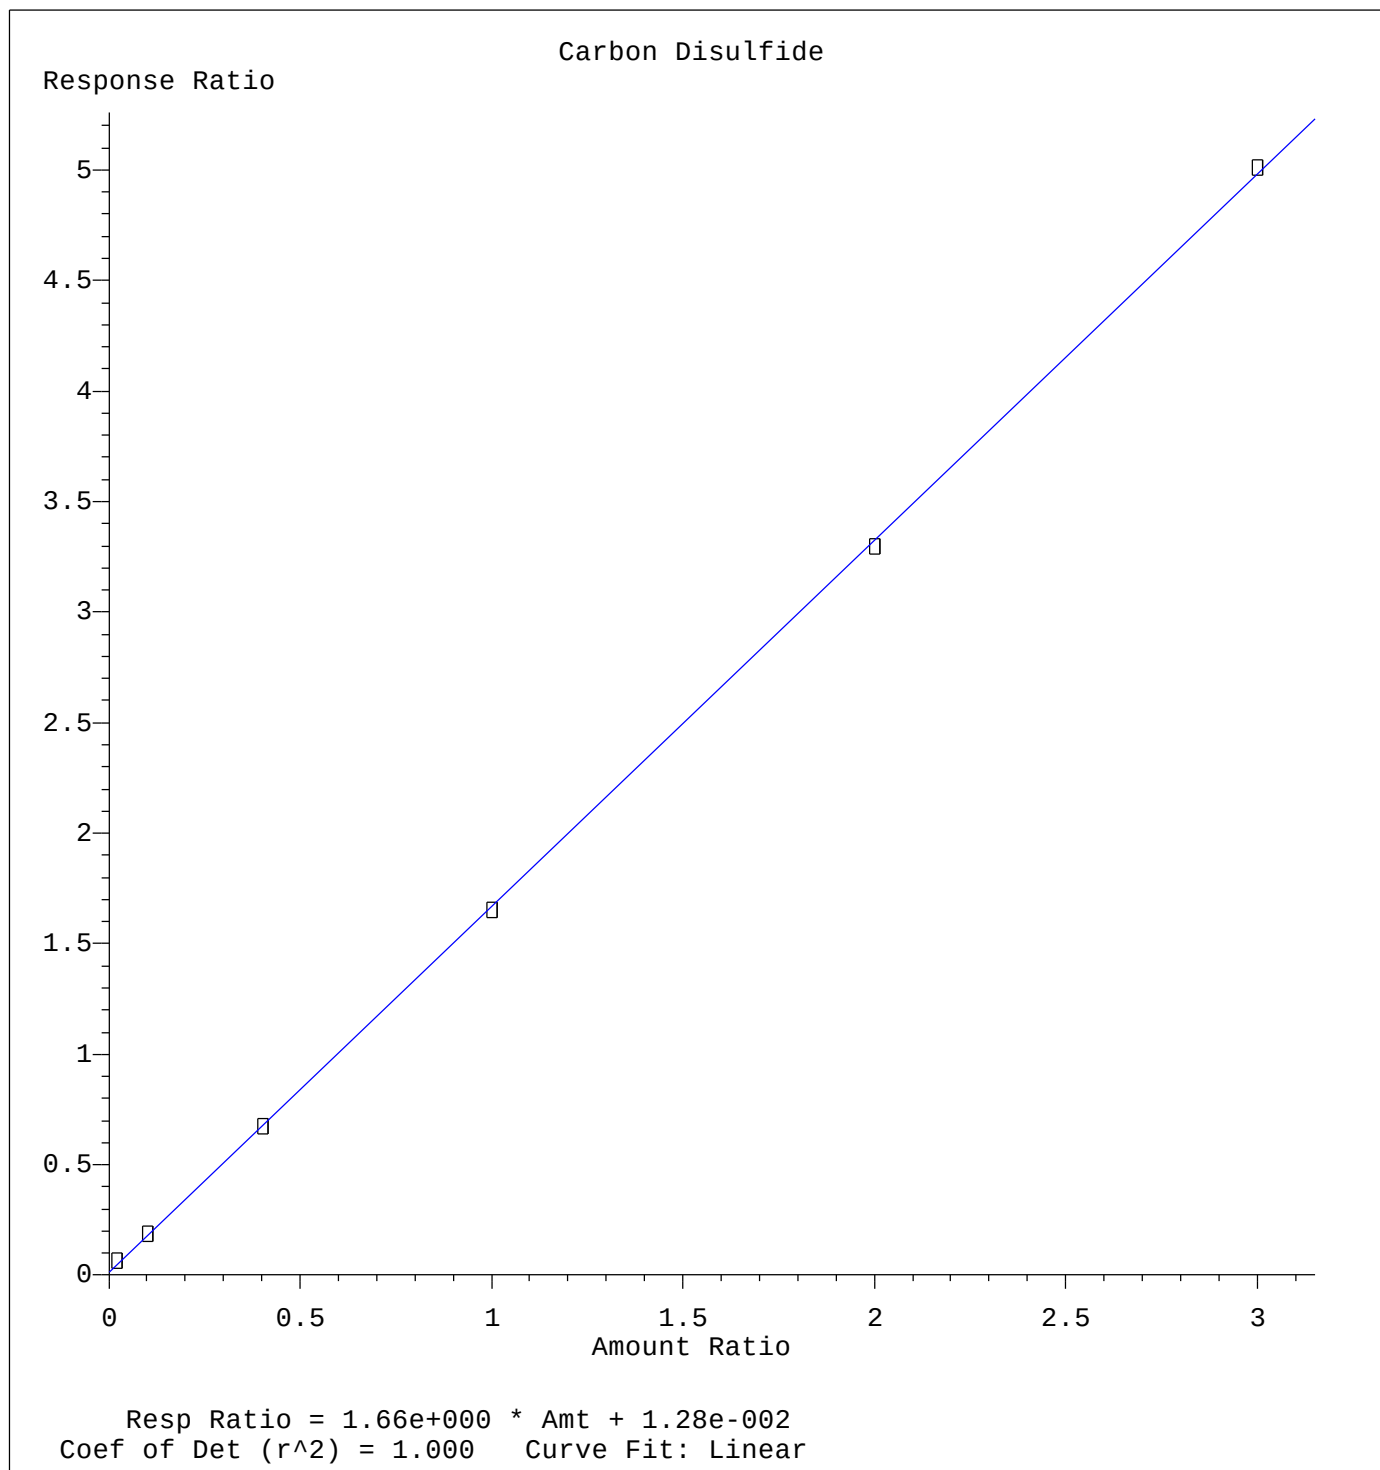

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X032519W.M
Calibration Table Last Updated: Tue Mar 26 07:57:20 2019

Methylene Chloride

Response Ratio

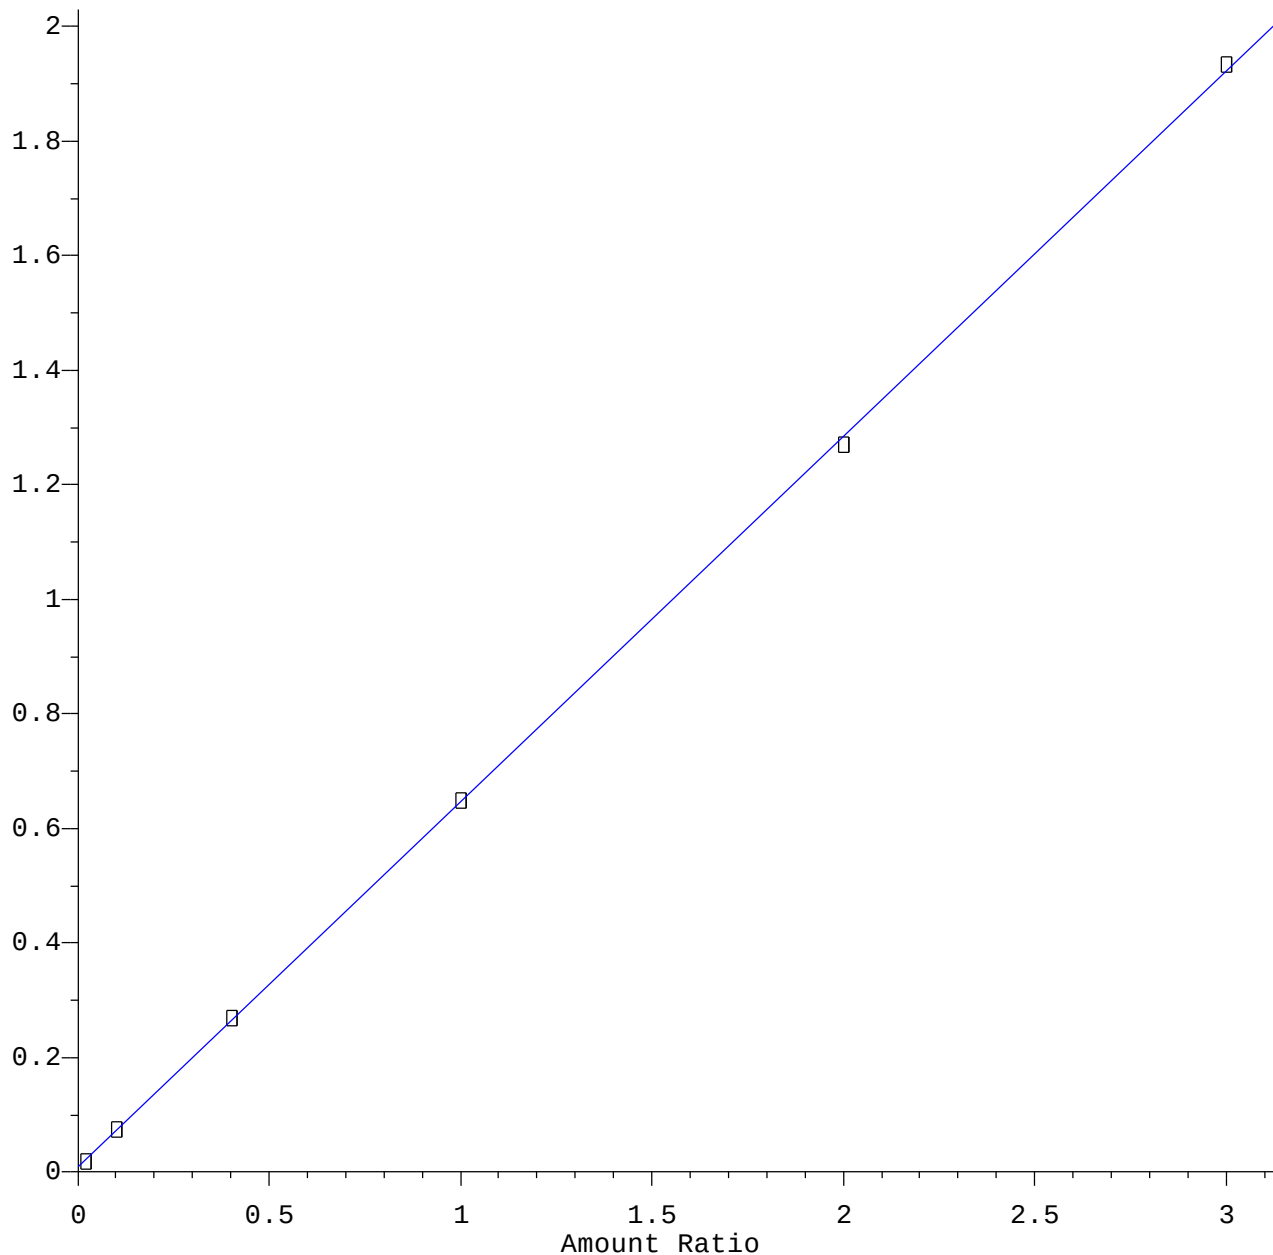


Resp Ratio = 6.38e-001 * Amt + 8.27e-003
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X032519W.M
Calibration Table Last Updated: Tue Mar 26 07:57:20 2019


trans-1,2-Dichloroethene

Response Ratio

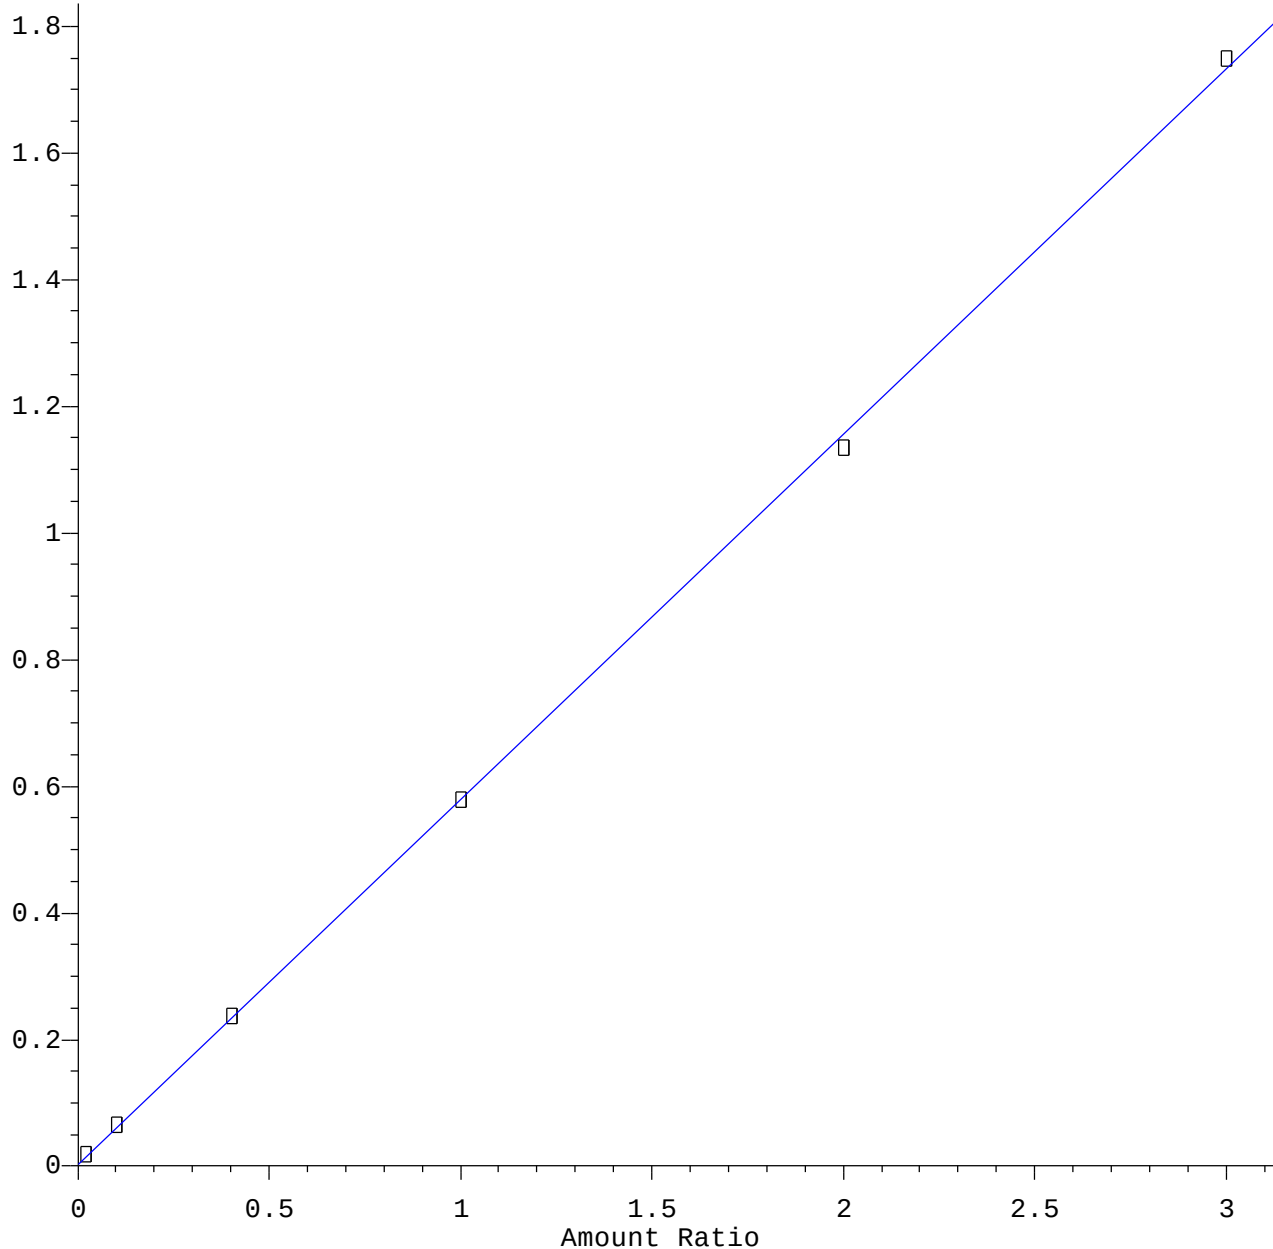

Resp Ratio = $5.76 \times 10^{-1} \times \text{Amt} + 3.14 \times 10^{-3}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X032519W.M
Calibration Table Last Updated: Tue Mar 26 07:57:20 2019

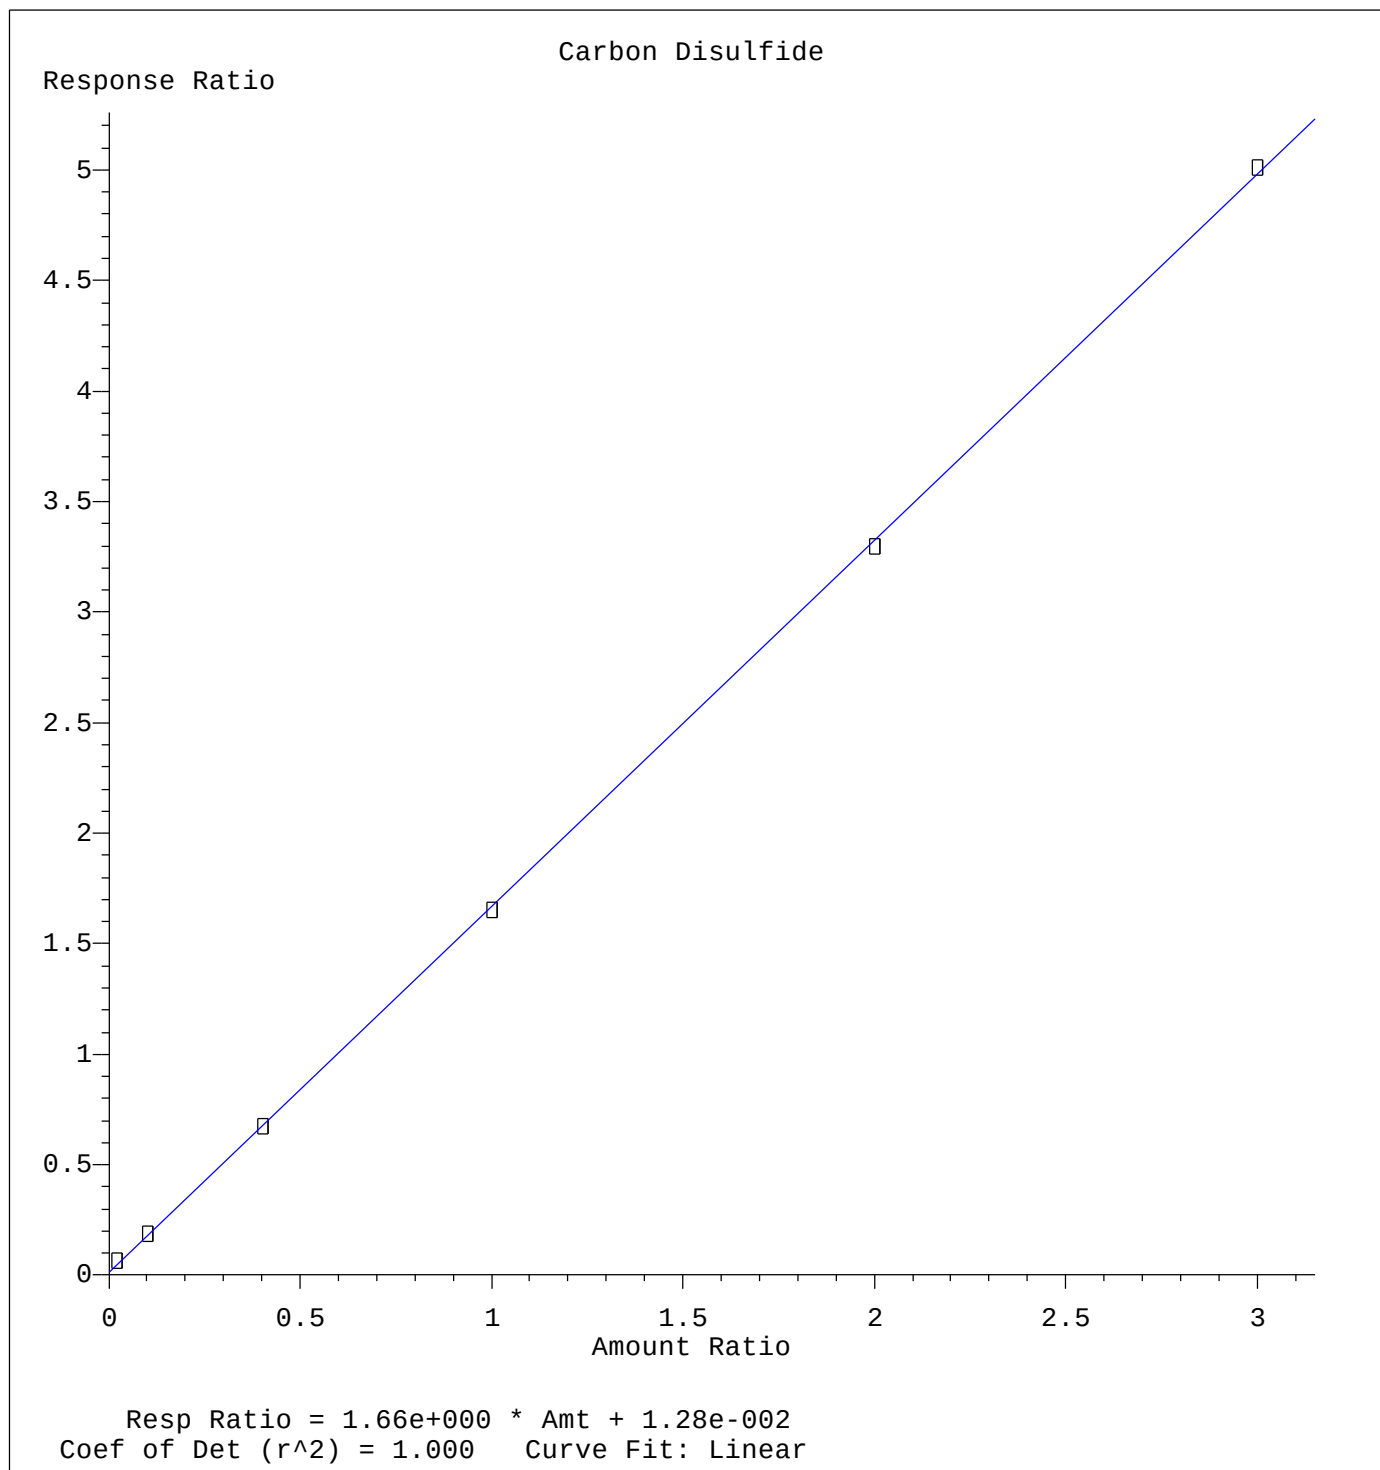

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X032519W.M
Calibration Table Last Updated: Tue Mar 26 07:57:20 2019