


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX032519\
Data File : VX008407.D
Acq On : 25 Mar 2019 12:39
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X032519W.M
Title : SW846 8260
Last Update : Tue Mar 26 07:57:20 2019

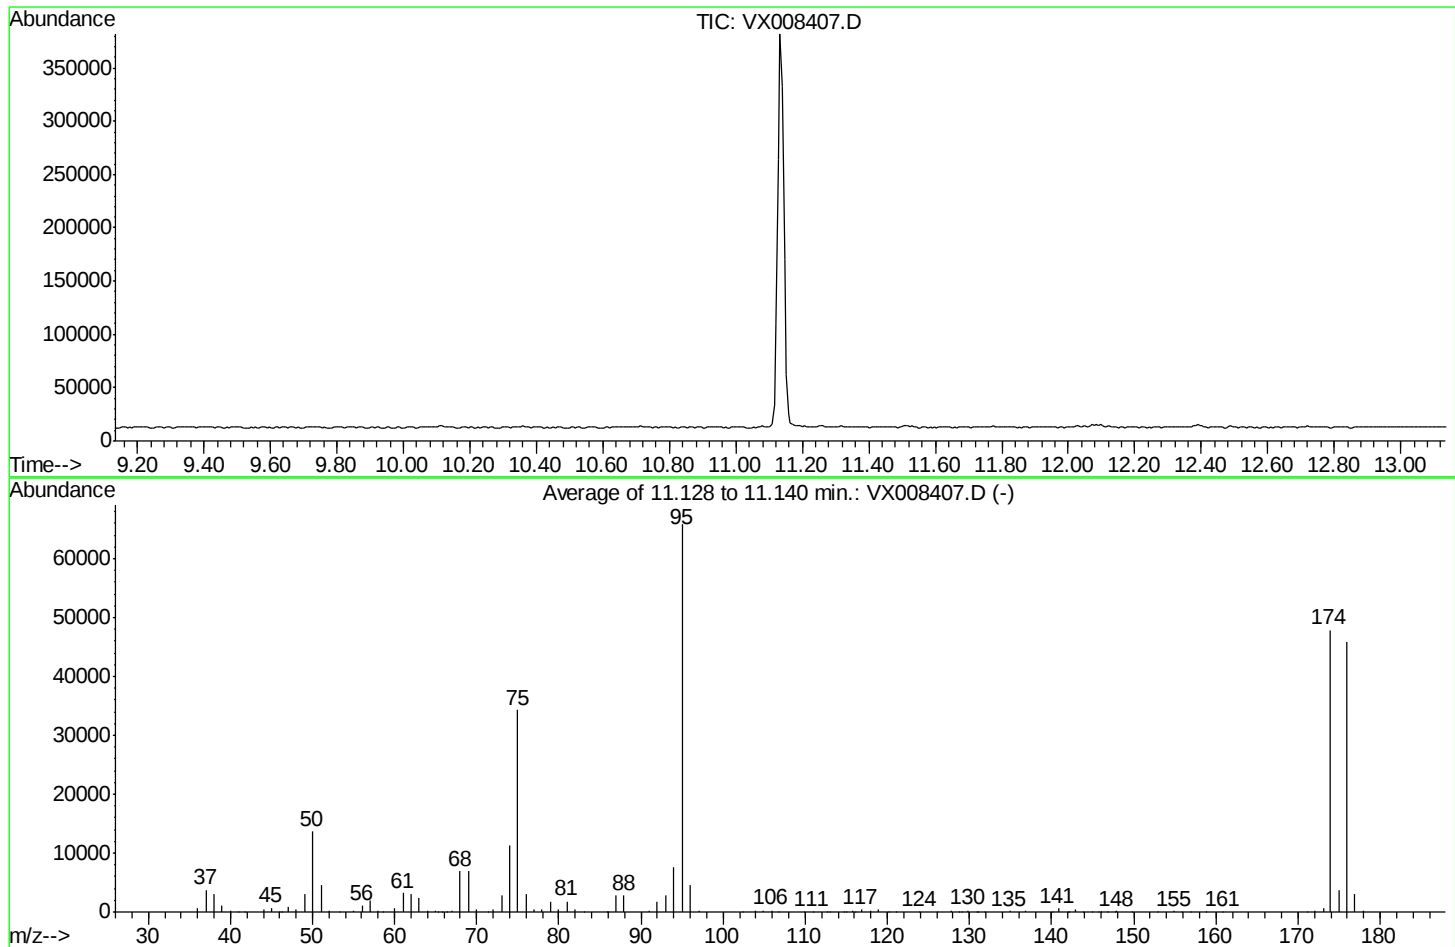

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	13604	PASS
75	95	30	60	52.2	34340	PASS
95	95	100	100	100.0	65826	PASS
96	95	5	9	6.9	4521	PASS
173	174	0.00	2	1.3	618	PASS
174	95	50	100	72.8	47909	PASS
175	174	5	9	7.7	3679	PASS
176	174	95	101	95.6	45818	PASS
177	176	5	9	6.5	2960	PASS