


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX032519\
Data File : VX008418.D
Acq On : 25 Mar 2019 18:12
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X032519W.M
Title : SW846 8260
Last Update : Tue Mar 26 07:57:20 2019

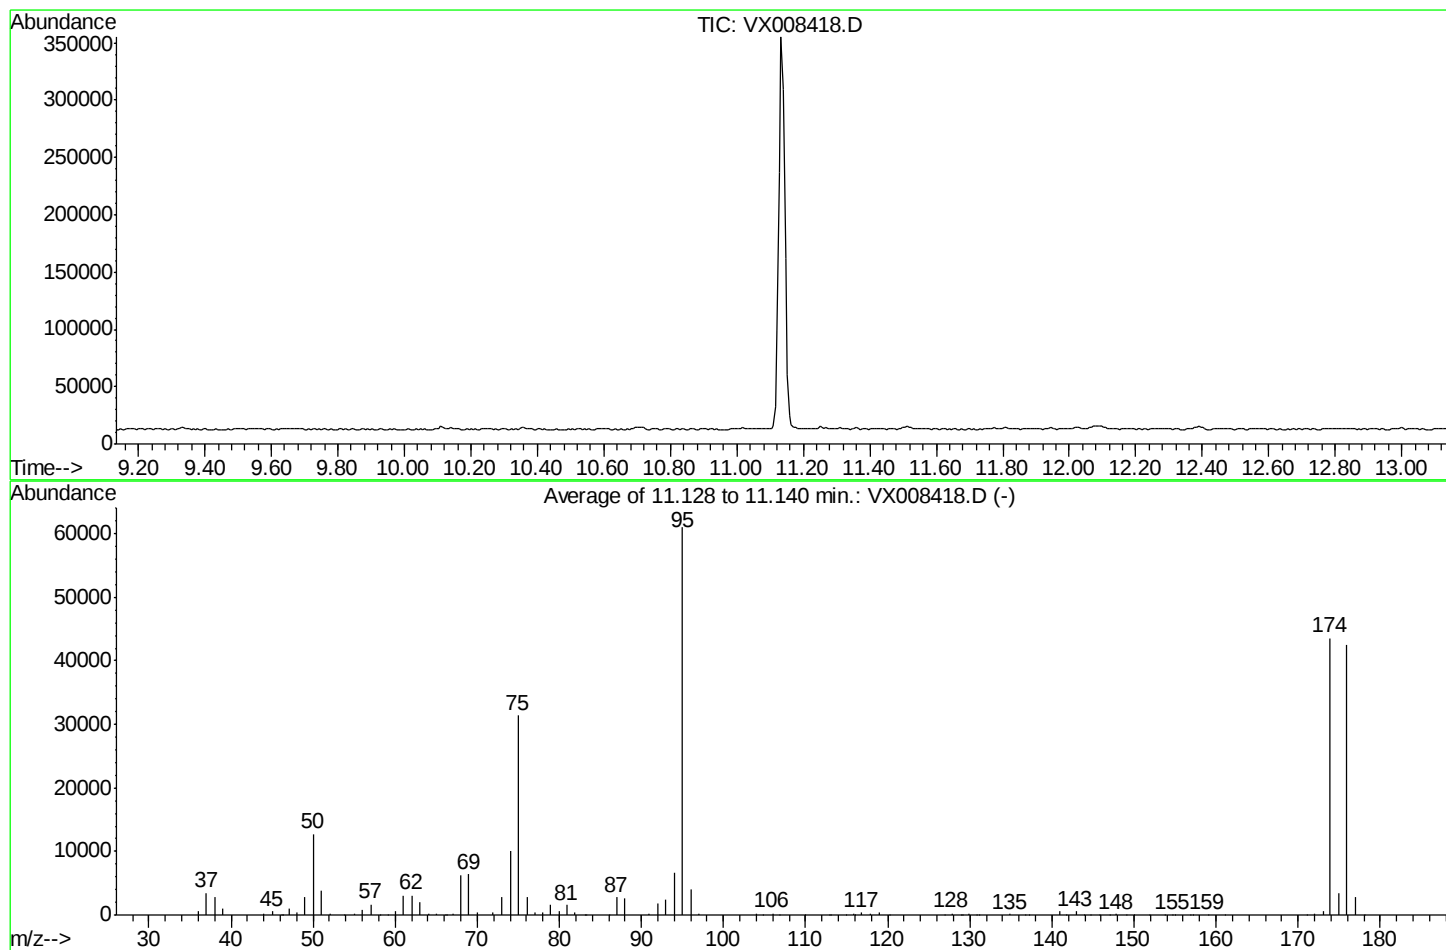

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	12724	PASS
75	95	30	60	51.5	31422	PASS
95	95	100	100	100.0	61005	PASS
96	95	5	9	6.5	3986	PASS
173	174	0.00	2	1.3	564	PASS
174	95	50	100	71.4	43544	PASS
175	174	5	9	7.7	3351	PASS
176	174	95	101	97.6	42480	PASS
177	176	5	9	6.7	2825	PASS