


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX032520\
 Data File : VX015345.D
 Acq On : 25 Mar 2020 17:01
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X032520W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Thu Mar 26 02:31:53 2020

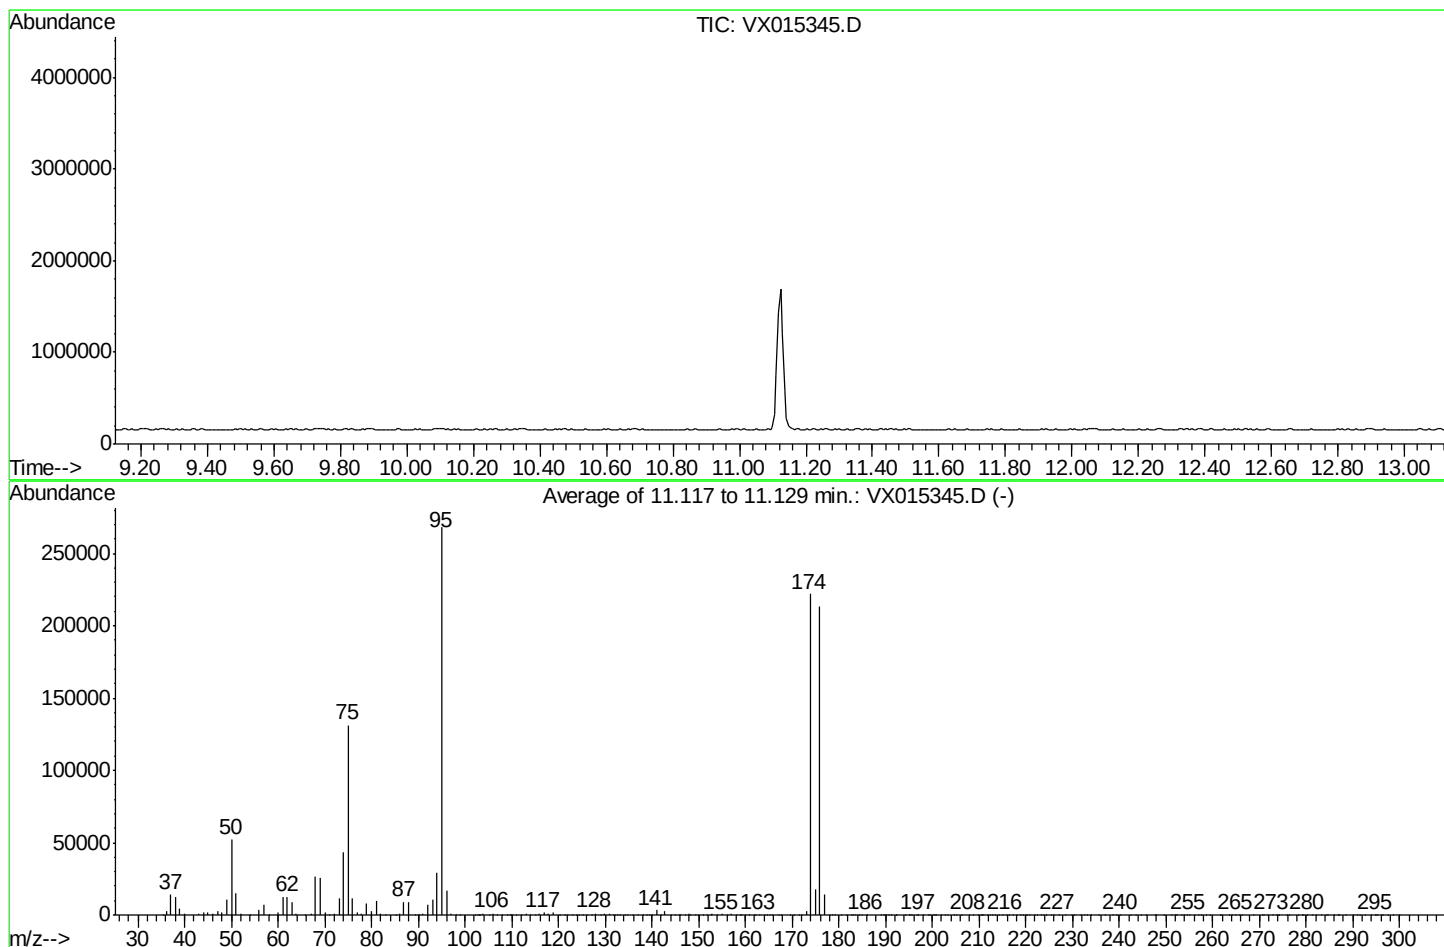

AutoFind: Scans 1678, 1679, 1680; Background Corrected with Scan 1672

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	51853	PASS
75	95	30	60	48.9	131212	PASS
95	95	100	100	100.0	268082	PASS
96	95	5	9	6.1	16453	PASS
173	174	0.00	2	1.2	2615	PASS
174	95	50	100	82.8	222052	PASS
175	174	5	9	8.0	17676	PASS
176	174	95	101	96.2	213557	PASS
177	176	5	9	6.5	13888	PASS